

First-in-human pilot study of snapshot multispectral endoscopy for early detection of Barrett's-related neoplasia

Dale J Waterhouse^{1,2}, Sophia Bano², Wladyslaw Januszewicz³, Dan Stoyanov², Rebecca C Fitzgerald⁴,

Massimiliano di Pietro^{4*} and Sarah E Bohndiek^{1*}

- 5 1. Department of Physics and Cancer Research UK Cambridge Institute, University of Cambridge, UK
2. Wellcome / EPSRC Centre for Interventional and Surgical Sciences, University College London, UK
3. Department of Gastroenterology, Hepatology and Clinical Oncology, Medical Centre for Postgraduate Education, Warsaw, Poland
4. MRC Cancer Unit, Hutchison/MRC Research Centre, University of Cambridge, UK

10

Co-corresponding Authors:

* Address correspondence to: Sarah E. Bohndiek

Department of Physics, Cavendish Laboratory, JJ Thomson Avenue, Cambridge, CB3 0HE, UK and Cancer Research UK Cambridge Institute, University of Cambridge, Li Ka Shing Centre, Robinson Way, Cambridge,

15 CB2 0RE, UK. e-mail: seb53@cam.ac.uk

* Address correspondence to: Massimiliano di Pietro

MRC Cancer Unit, University of Cambridge, Hutchison/MRC Research Centre, Box 197, Cambridge Biomedical Campus, Cambridge, CB2 0XZ, UK. e-mail: md460@mrc-cu.cam.ac.uk

20 **Grant Support**

DJW is supported by an EPSRC Doctoral Fellowship. WJ is funded by a Cancer Research UK multidisciplinary award (C47594/A21202). We would like to acknowledge the support of Cancer Research UK (C14303/A17197, C9545/A29580, C47594/A16267, C47594/A21102, C55962/A24669), EPSRC (EP/N014588/1, EP/R003599/1), the National Institute of Cancer Research, and the infrastructure support from the Experimental Cancer Imaging Centre and Cambridge Biomedical Research Centre.

Author Contributions

Study concept and design: DJW, MdP, RCF, SEB. Acquisition of data: DJW, MdP, WJ. Analysis of data: DJW,

30 SEB. Machine Learning: DJW, SB, DS. Drafting of the manuscript: DJW, SEB. Manuscript revision: All authors.

Conflict of Interest Statement

The authors have no conflicts of interest to declare.

35

Abstract

Significance: The early detection of dysplasia in patients with Barrett's esophagus could improve outcomes by enabling curative intervention, however, dysplasia is often inconspicuous using conventional white-light endoscopy.

40

Aim: We sought to determine whether multispectral imaging could be applied in endoscopy to improve detection of dysplasia in the upper gastrointestinal (GI) tract.

45

Approach: We used a commercial fiberscope to relay imaging data from within the upper GI tract to a snapshot multispectral imaging camera capable of collecting data from 9 spectral bands. The system was deployed in a pilot clinical study of 20 patients (ClinicalTrials.gov NCT03388047) to capture 727 *in vivo* image cubes matched with gold-standard diagnosis from histopathology. We compared the performance of seven learning-based methods for data classification, including linear discriminant analysis, k-nearest neighbor classification and a neural network.

50

Results: Validation of our approach using a Macbeth color chart achieved an image-based classification accuracy of 96.5%. Although our patient cohort showed significant intra- and inter-patient variance, we were able to resolve disease specific contributions to the recorded multispectral imaging data. In classification, a combined principal component analysis and k-nearest neighbor approach performed best, achieving accuracies of 95.8%, 90.7% and 76.1% respectively for squamous, non-dysplastic Barrett's esophagus (NDBE) and neoplasia based on majority decisions per-image.

55

Conclusions: Multispectral imaging shows promise for disease classification in Barrett's esophagus and merits further investigation as a tool in high-definition 'chip-on-tip' endoscopes.

60

Keywords

multispectral; endoscopy; dysplasia; computer assisted diagnosis

Introduction

Patients with Barrett's esophagus¹ (BE) undergo routine surveillance using high-resolution white light endoscopy (HR-WLE) and random biopsies to detect the presence of dysplasia, which increases the risk of developing esophageal adenocarcinoma². Early detection of the pre-cursor dysplastic lesions, or early-stage cancer, enables curative intervention, increasing the 5-year survival rate from just 15–25% to 80%^{3–5}. Unfortunately, these pre-cursor lesions can be challenging to identify on standard-of-care HR-WLE^{6,7}.

Advanced optical imaging modalities have potential to impact patient care⁸. With demand for endoscopy predicted to rise substantially over the next decade⁹, the unmet clinical need for optical methods with improved diagnostic yield and/or lower cost per procedure is particularly acute. When light travels through tissue, it is absorbed by endogenous chromophores, such as hemoglobin, and scattered by endogenous structures, such as cell nuclei¹⁰. Disease-related structural and biochemical changes in the epithelial layer of the gastrointestinal tract can alter the distribution and abundance of these absorbers and scatterers — for example, neovascularization increasing hemoglobin abundance in the epithelium¹¹ — resulting in subtle wavelength-dependent changes in reflected light, which can be measured by point-based spectroscopy methods¹², but also by hyperspectral imaging methods that capture spatially resolved (x, y) and spectral (wavelength, λ) information in a single data set, often using mechanical scanning^{13,14}.

Multispectral imaging (MSI) represents a compromise between the extremes of point-spectroscopy and hyperspectral imaging, providing typically up to 10 wavelengths of information, which can be sufficient to resolve color features, while requiring generally simpler optics and enabling faster scan times. HR-WLE actually represents a simple case of MSI, where tissue features are measured in three broad color bands: red (620 ± 40 nm), green (540 ± 40 nm) and blue (470 ± 40 nm) to replicate the spectral sensitivity of human vision¹⁵. Though this represents a substantial improvement over monochrome imaging, finer spectral information is lost as the light is pooled into three broad bands. More recently, narrow band imaging¹⁶ (NBI) was developed specifically to enhance contrast for vasculature and superficial mucosal morphology, using two narrow illumination bands (415 ± 10 nm and 540 ± 10 nm). Similarly, blue-light imaging uses a narrow band of blue light (410 ± 10 nm) to improve the contrast of vessels and mucosal pits¹⁷. In combination with data analysis using spectral unmixing algorithms, multispectral and hyperspectral imaging have been used in a range of biomedical applications: to visualize the vascular pattern and

the oxygenation status of blood^{18–26}; to improve detection of gastric²⁷ and colorectal lesions^{28–30}; for intraoperative
90 image guidance³¹; to identify residual tumour³²; and to perform tissue segmentation^{33,34}.

The majority of multispectral imaging devices fall into two categories: amplitude-division, where the light beam is divided into two new beams; and field-division, where the light is filtered or divided based on its position in the beam³⁵. With all multispectral imaging approaches, a trade-off between spatial, spectral, and temporal resolution, must be considered alongside cost, complexity, size, and robustness. Previously reported spectral
95 endoscopy systems generally use amplitude-division, including multiple bandpass filters^{29,36}, tunable filters^{28,37}, laser lines^{38–40}, or detectors dedicated to separate spectral bands^{38,39}. These amplitude-division systems are typically bulky, costly, and more susceptible to misalignment in a clinical environment. Furthermore, they often require sequential acquisition resulting in slow acquisition rates, unsuitable for real-time clinical imaging. Several field-division approaches are available, including line-scanning⁴¹ and image mapping spectroscopy²⁰. Spectrally resolved
100 detector arrays (SRDAs) are a relatively new addition^{18,42,43}, exploiting spectral filters deposited directly onto the imaging detector in a mosaic pattern to achieve a low-cost, compact and robust device that is well suited to clinical application.

Here, we sought to determine whether multispectral imaging using an SRDA could be applied in endoscopy to improve detection of dysplasia in the upper gastrointestinal (GI) tract in patients with BE. We created a custom
105 MSI endoscope and undertook a first-in-human pilot clinical study to acquire *in vivo* MSI data from esophageal tissue matched with gold-standard histopathological diagnosis of disease state. These data were then subjected to machine learning-based classification methods, indicating that despite substantial intra- and inter-patient variation, MSI has the potential to resolve different esophageal disease states in patients with BE.

|10 **Methods**

A snapshot multispectral endoscope for in vivo clinical imaging

SRDAs could in future be deployed as ‘chip-on-tip’ cameras at the distal end of an endoscope, however, such integration requires significant miniaturization of optics and changing a clinically approved device, which substantially extends the timeline required for first-in-human testing. Furthermore, the spectral properties of |15 esophageal tissue are not well characterized, nor reliably measured using *ex vivo* tissue⁴⁴. Thus, to facilitate clinical testing, we combined the SRDA with a CE-marked ‘babyscope’ (PolyScope, PolyDiagnost, Germany), a small fiber-bundle-based endoscope that can be inserted through the accessory channel of a standard endoscope to relay light between external optics and the esophageal lumen. We have previously shown that SRDAs can be implemented in combination with such an imaging-fiber bundle without reducing resolution, since the resolution of fiberscope-based imaging is limited by the size of individual fiberlets rather than by the sensor resolution⁴⁵. The babyscope |20 system included: a single fiber to relay illumination from outside the patient and direct it onto the tissue; and a 10,000-fiberlet imaging bundle to relay diffusely reflected light from the esophageal tissue to custom external detection optics (**Fig. 1A**). The 3mm diameter of this babyscope allowed it to be introduced through the accessory channel of a therapeutic gastroscope (**Fig. 1B**). Utilizing this unmodified CE-marked device to relay light between |25 the esophagus and external optics facilitated clinical application of the spectral endoscope.

At the proximal end of the babyscope, the illumination fiber was coupled to a broadband supercontinuum light source (SuperK COMPACT, NKT Photonics, UK), which provided illumination from 450–875 nm (**Supplementary Fig. 1**). The proximal end of the imaging fiber was imaged and magnified using an objective lens (UPLFLN20x, Olympus, Japan). The light was split using a 90:10 plate beam splitter (BSN10R, Thorlabs, |30 Germany) and focused using an achromatic doublet lens ($f = 100$ mm, ACA254-100-A, Thorlabs, Germany); 10% of the light was focused onto a red-green-blue (RGB) camera (Grasshopper 3.0, IDS, Germany) to record reference images and the remaining 90% was focused onto the SRDA (CMS-V, SILIOS, France) (**Fig. 1C**). The SRDA consists of 9 spectral filters deposited as a 3×3 super-pixel (**Fig. 1D**) across a Complementary Metal Oxide |35 Semiconductor (CMOS) sensor (NIR Ruby sensor, UI1242LE-NIR, IDS, square pixel size 5.3 μm matched to spectral filter size). The 9 spectral filters comprises 8 narrow bands of average full width half maximum (FWHM) 30 nm with center wavelengths 553, 587, 629, 665, 714, 749, 791, 829 nm, along with 1 broad band; 500–850 nm (**Fig. 1E**). The optics were securely housed inside a light tight enclosure and mounted on an optical breadboard

(MB4545/M, Thorlabs, Germany), which was fixed to a stainless-steel trolley (FW2901-3, Freeway Medical, UK) with a footprint of 512 mm × 480 mm, allowing the system to be easily and safely transported in a busy and often crowded clinical setting.

This distal end of the multispectral endoscope accessed the esophagus via the working channel of a therapeutic gastroscope, directed by the articulation of the gastroscope to collect diffuse reflectance images alongside standard-of-care imaging (**Fig. 1F**), thus causing minimal disruption to clinical workflow.

Endoscope settings were controlled using an interface developed in LabVIEW (National Instruments, USA) running on a PC and a tablet (Surface Pro, Microsoft, USA). Images captured by the SRDA were saved as 8-bit 1280 x 1024-pixel bitmap image files (to enable fast acquisition and immediate review of the images). These images contain two artefacts: a comb structure due to the imaging fiber bundle and a mosaic pattern due to the spectral filters of the SRDA (**Fig. 2A**). For analysis, these were removed in a process of demosaicing and decombing as described previously⁴⁵, resulting in a 1280 pixel x 1024 pixel x 9 band image cube (**Fig. 2B**) with a spatial resolution of $240 \pm 20 \mu\text{m}$ at a working distance of 1 cm. For real-time display, 3 of the 9 bands were decombined and displayed as a false-RGB image at up to 15 fps. For analysis, columns of the image cube can be treated as 9-point ‘per-pixel spectra’ (**Fig. 2C**). As high-dimensional image data would be challenging for an operating clinician to interpret in real-time, machine-vision techniques can be used to classify per-pixel spectra to produce a tissue map for endoscopic image guidance (**Fig. 2D**).

Color chart imaging

To test the accuracy of the snapshot multispectral endoscope in a controlled setting with known reference data, we performed handheld imaging of a Macbeth color chart (ColorChecker Classic Mini, x-rite) prior to 4 of the *in vivo* trials (**Fig. 3**). The color calibration target consists of 24 squares of painted samples, 18 of which contain colors whose spectral reflectance is intended to mimic those found in natural objects and 6 of which are a uniform grey lightness scale.

First-in-human pilot study of snapshot multispectral endoscopy

The snapshot multispectral endoscope was deployed in a pilot clinical study to acquire *in vivo* images. This prospective pilot cohort study was carried out at the Cambridge Clinical Research Centre, Cambridge University

Hospitals, UK. Eligible patients were adults (at least 18 years old) with a previous diagnosis of BE with an endoscopic length of at least 2 cm if circumferential (circumferential extent C \geq 2 according to the Prague classification) or at least 3 cm if not circumferential (maximal extent M \geq 3 according to the Prague classification). Exclusion criteria are given in the **Supplementary Materials**. The trial was reviewed by Cambridgeshire Research Ethics Committee and was approved in March 2018 (18/NW/0134). The trial was registered at ClinicalTrials.gov (NCT03388047).

Endoscopic procedure and histopathology

The clinical procedure undertaken is summarized in **Supplementary Fig. 2**. Each procedure was performed

by a single experienced endoscopist (MdP).

- i. After local anesthesia and/or conscious sedation (Midazolam \pm Fentanyl) the patient was intubated with HR-WLE (H290Z, Olympus, Japan). After cleaning the esophageal mucosa using a water jet, the endoscopist thoroughly inspected the mucosal surface of the esophagus. Cautery marks were placed around two regions of interest: one suspicious lesion and one region of inconspicuous BE as a control. In the absence of suspicious lesions one or more random areas within the BE segment was selected depending on the length of the BE. The HR-WLE video stream was recorded using a recording unit (SMP300, Extron, USA).
- ii. The endoscopist inserted the snapshot multispectral endoscope through the working channel of a therapeutic endoscope (GIF2T240, Olympus, Japan). The use of the therapeutic scope was required as its accessory channel was sufficiently large (3.7 mm diameter) to allow easy insertion of the multispectral endoscope (3.0 mm diameter at tip, 2.65 mm along length). The multispectral endoscope was used to image the regions of interest cautery marked in step (i). An endoscope cap was not used as it can easily come into contact with lesions and induce contact bleeding. For the second half of the trial (trial number 11 onwards), an additional control region of distant squamous tissue was inspected with the multispectral endoscope following inspection of the two marked regions.
- iii. The multispectral endoscope was withdrawn and the endoscopist proceeded to an endoscopic mucosal resection or biopsy (depending on the endoscopic findings and the level of suspicion). Control areas

195 received biopsies only. Pathological assessment of biopsies was performed by an expert GI pathologist with extensive experience in reporting BE-related neoplasia⁴⁶⁻⁴⁸. Histopathology was interpreted according to the revised Vienna classification⁴⁹. In case of dysplasia, a second pathologist reviewed the diagnosis to achieve consensus.

200 For analysis, the most advanced disease present in each biopsy determined the label for the region such that 3 classes of spectra were acquired: (1) normal squamous; (2) non-dysplastic BE (NDBE); and (3) neoplasia (consisting of dysplasia and intramucosal carcinoma).

Coregistration of multispectral images with diagnosis from histopathology

205 To enable matching of multispectral image data with the diagnosis from histopathology, the HR-WLE video stream and the video stream from the multispectral endoscope were synchronized and placed side-by-side for analysis. The HR-WLE video was carefully inspected to extract frames where the multispectral endoscope was sampling the marked regions of interest that were biopsied to give gold-standard diagnosis from histopathology. Since the esophageal lumen is quite featureless on multispectral imaging, frames were identified using the cautery marks and other visible landmarks in the HR-WLE video stream to estimate the field of view of the multispectral endoscope. The tip of the multispectral endoscope was visible within the field of view of the HR-WLE endoscope, which facilitated identification of appropriate multispectral images that could be related to the gold-standard diagnosis made by histopathology.

Spectral data processing

215 Briefly, raw images were checked for saturation (pixel values>250), dark subtracted then decombed, to account for the structure introduced to the image by the individual fiberlets, and demosaiced, to separate the 9 spectral bands, creating an image cube as outlined previously⁴⁵. In the image cube, low signal pixels were removed (max per-pixel spectrum value<50) as they are more likely to be affected by noise. Finally, each per-pixel spectrum was divided by a white light reference spectrum and normalized to the maximum of the per-pixel spectrum, such that the per-pixel spectra represent max-normalized reflectance. The white reference spectrum was an average of

?20 images captured from a white reflectance standard prior to each procedure to avoid variations introduced depending on experimental conditions.

For classification, the spatial dimensions were binned into 32 x 32 pixels as a compromise between retaining spatial information and increasing classification accuracy by reducing noise (**Supplementary Fig. 3**). This resulted in 40-pixel x 32-pixel x 9-band multispectral image cubes. Each multispectral image cube therefore contains 1,280
?25 9-band spectra. By averaging these across a region of interest drawn in the center of the image around the center of the fiber bundle, a mean spectrum was determined for each image (this occurs prior to reflectance normalization such that brighter pixels contribute more to the mean image spectrum). By averaging the spectra across images of the same tissue type within a given patient, mean ‘patient spectra’ were determined. These different categories enabled us to test the performance of different classification methods on a per-pixel, per-image or per-patient basis.

?30 To quantify the variance in the data, standard deviations were calculated according to:

$$\sigma = \sqrt{\left(\frac{\sum_{\lambda=1}^9 \sum_{i=1}^n (y_{i,\lambda} - \bar{y}_{\lambda})^2}{n} \right)} \quad (\text{E1})$$

where $y_{i,\lambda}$ is reflectance i at band λ , with $i = 1: n$, the number of spectra and $\lambda = 1: 9$, the 9 bands of the spectrum, and \bar{y}_{λ} is the mean reflectance in band λ . This was calculated within each group (e.g. per-patient) and the average over all groups (e.g. all patients) was calculated using a simple mean. For example, for the standard deviation per-image within-patients:

$$\sigma_{\text{within-patient}} = \frac{\sum_{p=1}^N \sigma_p}{N} \quad (\text{E2})$$

?35 where σ_p is the standard deviation of all per-image spectra within patient p calculated according to **Equation 1** and N is the number of patients.

Classification of multispectral image cubes to discriminate tissue pathologies

For classification, the multispectral image cubes were randomly split into 80% for training and 20% for
?40 testing. Spectra calculated per-pixel and per-image were classified using 7 methods commonly used in spectral data classification⁵⁰. Linear discriminant analysis (LDA) classifies spectra by finding a linear combination of features that maximizes the separation between classes relative to within-class variance in the feature space. K-nearest neighbor (KNN) algorithms classify spectra by choosing the most frequent classes of k-nearest neighbor data points

in the feature space ($k = 3, 5$ and 7 were tested). Both LDA and KNN classifiers were applied using the 9-band
?45 spectrum directly as a 9-element feature vector. While LDA assumes linear decision boundaries, the KNN algorithm is non-parametric, so makes no assumptions about the shape of the decision boundaries. LDA also assumes variables are Gaussian distributed. The data were also projected onto principal component axes using principal component analysis (PCA) and the weights used for KNN classification. Spectral angle mapping (SAM) calculates the n-dimensional angle between a target spectrum and a reference spectrum; in this case $n=9$. The reference spectra are
?50 the mean spectra per-pathology within the training dataset; thus 3 spectral angles are calculated for each target spectrum — $\theta_{\text{target-squamous}}$, $\theta_{\text{target-NDBE}}$ and $\theta_{\text{target-neoplasia}}$. For a simple-SAM classification, the minimum of these three angles were taken as the predicted class. Alternatively, the angles were treated as a 3-element feature vector and classified using LDA or KNN.

Finally, a neural network (NN) was used for classification. NNs perform classification by passing an input
?55 vector, in this case a 9-band spectrum, through a series of artificial neurons, with each neuron outputting some non-linear function of its inputs with some weight that is adjusted during training. The output values of the final layer determine the classification. In contrast to LDA, NN classification does not make assumptions about the distribution of input data nor the shape of decision boundaries. The NN was implemented using a 2-layer feed-forward network, with a sigmoid transfer function in the hidden layer (10 neurons) and a linear transfer function in the output layer,
?60 using the Matlab (Mathworks, USA) ‘Neural Network Pattern Recognition app’. The 20% testing image cubes were randomly split into 50% for validation and 50% for testing (10% of all image cubes each). In summary, the 7 classification methods compared were: LDA, KNN, PCA-KNN, simple-SAM, SAM-LDA, SAM-KNN and NN.

Accuracy for per-pixel classification was calculated in 3 ways: per-pixel accuracy, the percentage of pixels
?65 classified correctly over all pixels; per-image accuracy, the average percentage of pixels classified correctly in an image; and majority-pixel-per-image, the percentage of correctly classified images based on a relative majority decision (plurality) of all pixels within an image (if there is a tie between two classes, the image was counted as incorrectly classified). Accuracy for per-image-spectrum was the percentage of correctly classified mean-image-spectra.

Results

?70 *Clinical study recruitment*

Between May 2018 and December 2019, a total of 20 subjects were recruited to this pilot clinical trial (**Supplementary Table 1**). All patients provided written informed consent. Of these, one subject was considered unfit for endoscopic procedure due to concomitant acute comorbidity and one was excluded as the visible lesion was too small for spectral imaging. Of the 18 subjects that underwent standard-of-care endoscopic procedures, 3 ?75 were excluded from analysis because of insufficient illumination for spectral imaging using the first prototype (n=2) and failure of the standard-of-care recording unit (n=1).

The multispectral endoscope was deployed to acquire *in vivo* esophageal image cubes. The study design prioritized the collection of image cubes matched to gold-standard diagnosis from histopathology (**Supplementary Fig. 1**). To do this, cautery marks were made in two distinct regions of the esophagus, one deemed suspicious and ?80 one a control (**Supplementary Fig. 2A**). The marked regions were inspected with the multispectral endoscope (**Supplementary Fig. 2B**) then the regions were biopsied (**Supplementary Fig. 2C**) and diagnosed based on the histopathologic analysis of the biopsies (**Supplementary Fig. 2D**).

Data was collected in 15 subjects at 44 distinct regions: 9 regions of squamous tissue, 24 regions of NDBE, 11 regions of neoplasia. Of the 35 BE tissue regions, 34 were confirmed with histopathological assessment from 45 ?85 collected samples (33 biopsies, 14 endoscopic mucosal resections). In patient number 12, the control region identified on endoscopy was diagnosed as dysplastic by histopathology, so spectra that were incidentally captured from another region of NDBE were taken as NDBE without confirmation from histopathology. Coregistration between imaging data and histopathological diagnosis was successful for 30 regions (20 NDBE, 10 neoplasia), yielding a total of 570 labelled image cubes for analysis, plus an additional 157 image cubes from 9 squamous ?90 regions (**Table 1, Supplementary Fig. 4**). The mean exposure time was 200 ± 50 ms. Multispectral imaging lengthened the procedure time by <10 minutes per trial (data captured for mean of 5.2 ± 1.5 mins per trial).

Machine learning enables classification of reference color spectra

To validate the performance of the snapshot multispectral endoscope, handheld imaging of a Macbeth color ?95 chart was performed prior to imaging of 4 patients, resulting in 568 image cubes totaling 46,459 spectra for per-

pixel classification (**Fig. 3A, B**). The mean spectra per-pixel show distinct shapes but with significant overlap (**Fig. 3C**). For classification, 454 image cubes (36,714 spectra) were used for training and 114 image cubes (9,745 spectra) were used for testing. Visualization of the training spectra by PCA shows clustering by color, but also demonstrate the overlap between classes (**Fig. 3D**). Despite this overlap, classification was possible with 89.5% accuracy on a per-pixel basis ($96.1 \pm 11.4\%$ mean \pm standard deviation per-image) and up to 99.1% when taking a majority decision per-image using PCA-KNN with $k = 3$ (**Fig. 4A**). On per-image-spectrum classification basis, the accuracy was 96.5%. As expected, per-pixel classification results for each color show that misclassification often occurred between similar shades (**Fig. 4B**) and at the edges of the illuminated area, where noise is more apparent (**Fig. 4C**). Examples of classified image cubes representing colors from the middle row of the Macbeth color chart are shown in **Fig. 4C**.

Spectra show promising differences between tissue types despite considerable intra- and inter-patient variation

We first evaluated the variance within our data. There is considerable variance amongst the spectra, per-pixel (**Fig. 5A**), per-image (**Fig. 5B**) and per-patient (**Fig. 5C**), but the average spectra across patients show clear differences among different histopathological categories (**Fig. 5D**). We therefore sought to better understand the nature of the variance in the dataset (**Fig. 6**). The variance over all per-patient spectra, and over all per-pixel spectra, increases with progression of disease (0.213, 0.246, 0.321 for per-patient spectra and 0.459, 0.474, 0.479 for per-pixel spectra in regions of squamous, NDBE and neoplasia respectively). This is likely due to the increasing heterogeneity of the diseased tissues compared to healthy squamous tissue. Interestingly, the per-image variance within-patients is largest in NDBE. This might be due to intra-patient heterogeneity as multiple distinct regions of NDBE were imaged in 4 of the patients. It might also reflect the mosaic of cell types found in NDBE. The overall variance of spectra calculated per-image is smaller than the overall variance in the per-pixel spectra (0.226 vs. 0.459, 0.385 vs. 0.474, 0.276 vs. 0.479 for squamous, NDBE and neoplasia respectively), perhaps due to noise removal by averaging in the images (**Fig. 6A**). The same effect can be observed in PCA plots, where the spectra per-pixel (**Fig. 6B**) cluster less well than the spectral per-image (**Fig. 6C**). Spectra per-pixel and spectra per-image cluster by pathology (**Fig. 6B and C**) and by patient (**Fig. 6D and E**), which suggests significant inter-patient differences in the dataset, further supported by the standard deviation calculations (**Fig. 6A**). The within-patient variance in per-image spectra is smaller than the total variance (0.180 vs. 0.226, 0.227 vs. 0.385, 0.192 vs. 0.276 for squamous,

NDBE and neoplasia respectively), suggesting there are notable inter-patient differences, which would make
325 generalizable classification challenging.

Snapshot multispectral endoscopy shows promising accuracy for in vivo tissue classification

For classification, the patient data were split into training data comprising of 581 multispectral image cubes
(121,600 spectra) and test data comprising of 146 image cubes (31,405 spectra). Seven classification methods were
330 compared (**Fig. 7A**). Despite the substantial aforementioned variance in the dataset, classification per-pixel was
possible with 74.2% accuracy ($71.2 \pm 20.2\%$ mean \pm standard deviation per-image), rising to 87.0% accuracy when
taking a majority pixel decision per-image using PCA-KNN with $k = 3$ (**Fig. 7A**). Per-image-spectrum classification
increased accuracy to 96.5%. The classification results for each pathology show that squamous tissue was most
reliably classified, whilst neoplasia was most difficult to classify (**Fig. 7B**). This is in line with our expectations
335 given the variance described in the dataset, as well as the familiar clinical challenge of distinguishing neoplasia.
Nevertheless, on majority-pixel-per-image classification, accuracies of 95.8%, 90.7% and 76.1% were achieved
respectively for squamous, NDBE and neoplasia respectively and on per-image-spectrum classification, these rose
to 95.8%, 98.6% and 95.5% respectively. Confusion matrices are shown alongside calculated values of sensitivity,
specificity, positive predictive value and negative predictive value for neoplasia classification in **Supplementary**
340 **Fig. 5 and Supplementary Table 2.**

We then created classification maps representing the three pathologies (**Fig. 7C**) to display alongside RGB
images, composed by assigning bands 2, 3 and 9 (broadband) to red, green and blue respectively. For visualization,
map pixels whose four nearest neighbor pixels are all a different class (to the said pixel) are defined as noise and
replaced by the mode class of the four nearest neighbor pixels. The maps illustrate how classification data could be
345 presented to an operating endoscopist in real-time.

To calculate sensitivity, specificity, positive predictive value and negative predictive value for detection of
neoplasia in Barrett's esophagus, the classification models were retrained for 2-way classification using only NDBE
and neoplastic image cubes (**Supplementary Fig. 6, Supplementary Table 3**). For per-pixel classification PCA-
KNN with $k=3$ achieved 60.7% sensitivity, 88.1% specificity, 71.7% positive predictive value and 81.8% negative
350 predictive value. In per-image-spectrum classification, this increased to 97.7% sensitivity, 100% specificity, 100%
positive predictive values and 98.6% negative predictive value.

Discussion

Advanced optical imaging modalities have potential to impact the care of patients with BE, by enhancing contrast for early lesions that can be treated using minimally invasive endoscopic therapy. MSI enables both spatial and spectral information to be captured during endoscopy, which has the potential to achieve this goal by revealing changes in the distribution of optical absorbers and scatterers between different disease states. Diffusely reflected light collected in our multispectral endoscope is estimated to penetrate approximately $200 \pm 100 \mu\text{m}$ into tissue⁵¹, thus sampling the superficial mucosal layers where angiogenesis occurs in disease progression. We expect new microvessels to form from the pre-existing vascular network in the lamina propria and infiltrate the epithelium¹¹, increasing the hemoglobin abundance in the region sampled by our endoscope. Changes in cell and organelle morphology and arrangement might also contribute to changes in scattering in the epithelial layers^{52,53}.

To test the potential of MSI we constructed and tested in a pilot clinical study an SRDA-based snapshot multispectral endoscope capable of acquiring of 9-band multispectral image cubes *in vivo*. The SRDA-based snapshot multispectral endoscope was compatible with the clinical environment: it was deployed via the working channel of the standard-of-care endoscope allowing simultaneous standard-of-care imaging, illumination, articulation, insufflation and washing capabilities; its deployment lengthened procedure time by less than 10 minutes (data captured for mean of 5.2 ± 1.5 mins per trial); it was compact ($512 \text{ mm} \times 480 \text{ mm}$ footprint) and mobile, enabling it to be easily transported between procedure rooms between trials; and it was robust, allowing it to be used in a clinical setting with minimal realignment needed between trials.

Multispectral image cubes were successfully collected in 15 patients. Following multispectral imaging, biopsies were collected from the imaged regions, resulting in matched labelling from gold-standard diagnosis from histopathology. This resulted in the successful acquisition of 727 multispectral image cubes labelled with histopathological diagnosis from 39 distinct regions within 15 patients.

We found substantial intra- and inter-patient variation, which is likely due to the intrinsic spatial heterogeneity of the disease. In regions with diagnosis of multifocal disease, it is likely that some acquired image cubes include contributions from both focal neoplasia and the surrounding ‘sea’ of NDBE, which was not possible to mitigate in the present study. The challenge of coregistering small scale disease heterogeneity with *in vivo* imaging data has not yet been solved; as image segmentation becomes more detailed, so the co-registration of the

image field with histopathology becomes more challenging. Careful consideration of these issues should be made
380 in future studies aiming to use advanced spectral endoscopy methods to aid in Barrett's esophagus surveillance. Additional variance could be attributed to variations in imaging geometry caused by peristalsis and the position of the lesion, though normalization should mitigate this effect. Nevertheless, the average spectra across patients showed clear differences between pathologies.

Seven classification methods were trained to classify the data as squamous tissue, NDBE or neoplasia.

385 PCA-KNN was found to provide the best performance in our dataset, classifying pathology with 74.2% accuracy per-pixel ($71.2 \pm 20.2\%$ mean \pm standard deviation per-image), with majority pixel decision per-image achieving 87.0% accuracy and per-image-spectrum classification achieving 96.5% accuracy. Notably, 2-way per-image-spectrum classification of neoplasia was possible with 99.1% accuracy (sensitivity 97.7%, specificity 100%, negative predictive value 98.6%), which compares favorably with the American Society for Gastrointestinal
390 Endoscopy Preservation and Incorporation of Valuable Endoscopic Innovations (PIVI)⁵⁴ requirements for recommendation in BE surveillance⁵⁵ — per-patient sensitivity of $\geq 90\%$, negative predictive value $\geq 98\%$ and specificity $\geq 80\%$ for detecting high-grade dysplasia or early esophageal adenocarcinoma — and with other emerging optical methods for endoscopic surveillance of Barrett's esophagus⁸. If these results are validated with a per-patient analysis in a larger patient cohort, multispectral endoscopy could be incorporated to clinical practice to
395 improve the standard-of-care.

While these results are very promising, this first experience of applying an SRDA-based multispectral endoscope in patients revealed several limitations that will inform future work. Firstly, our classification algorithms were tested using a random per-image split. Future work with a larger dataset should employ a per-patient split on a dedicated test set to assess the classification performance when dealing with unseen patients, particularly in light
400 of the large inter-patient variation seen in this trial.

Secondly, our system was constructed using a commercial SRDA, selected for the even distribution of spectral bands across the near-infrared window of biological tissue. Though our findings are promising, the sensor was not optimized for the detection of disease-specific spectral signatures and the 9-band spectra of NDBE and neoplasia showed significant overlap. The spectral bands available on the SRDA in future studies could be

105 customized using recently reported fabrication processes^{56,57} and tailored to detection of specific disease signatures using spectral band optimization⁵⁸.

A third limitation of our multispectral endoscope is the use of an imaging fiber bundle to carry light to detectors outside the body. Though this afforded us a swift route to clinical translation, it limits acquisition to 10,000 spatial points per image cube and consequently, images are of low quality in comparison to the high-definition
110 images captured by standard of care endoscopes. Additionally, attenuation due to the imaging fiber bundle also decreases sensitivity. This is worsened by the low sensitivity of the SRDA, partly due to the low quantum efficiency of the underlying sensor (<60%) and partly due to the low transmission of the deposited spectral filters (~40%). For future studies and in the pathway to clinical adoption, the SRDA technology, customized as discussed above, would be most advantageous as a ‘chip-on-tip’ device at the distal end of the endoscope, which would immediately
115 overcome these limitations.

In summary, by combining the snapshot multispectral endoscope with machine learning techniques, we demonstrated a 74.2% accuracy per-pixel and 96.5% accuracy per-image for classifying squamous, NDBE and neoplasia in a first-in-human trial. The next steps are to expand this work by testing custom SRDAs tailored to disease-specific spectral signatures. With further testing, multispectral endoscopy has the potential to improve
120 detection of neoplasia during surveillance of Barrett’s esophagus.

Acknowledgments

This study would not have been possible without hard work of the staff of the Cambridge Clinical Research Centre and the infrastructure support of the NIHR Cambridge Biomedical Research Centre. Many thanks to Tara Evans for
125 her help in recruitment for this study. We would also like to thank Maria O’Donovan for her work in histopathology. The authors would like to express our deepest gratitude to those patients who agreed to take part in this study, without whom this research would not have been possible.

Code, Data and Materials Availability

130 All code and data associated with this manuscript will be made available upon publication of the paper through the University of Cambridge Data Repository through a directly addressable DOI.

135 **References**

1. Y. Peters et al., "Barrett oesophagus," *Nat. Rev. Dis. Prim.* **5**(1), Springer US (2019) [doi:10.1038/s41572-019-0086-z].
2. P. Gatenby et al., "Lifetime risk of esophageal adenocarcinoma in patients with Barrett's esophagus.," *World J. Gastroenterol.* **20**(28), 9611–9617 (2014) [doi:10.3748/wjg.v20.i28.9611].
- 140 3. P. C. Enzinger and R. J. Mayer, "Esophageal cancer.," *N. Engl. J. Med.* **349**, 2241–2252 (2003).
4. A. Pennathur et al., "Esophagectomy for T1 Esophageal Cancer: Outcomes in 100 Patients and Implications for Endoscopic Therapy," *Ann. Thorac. Surg.* **87**(4), 1048–1055, The Society of Thoracic Surgeons (2009) [doi:10.1016/j.athoracsur.2008.12.060].
- 145 5. A. Pennathur et al., "Oesophageal carcinoma," *Lancet* **381**(9864), 400–412, Elsevier Ltd (2013) [doi:10.1016/S0140-6736(12)60643-6].
6. S. J. Spechler et al., "American Gastroenterological Association technical review on the management of Barrett's esophagus.," *Gastroenterology* **140**(3), e18–e52 (2011) [doi:10.1053/j.gastro.2011.01.031].
7. R. C. Fitzgerald et al., "British Society of Gastroenterology guidelines on the diagnosis and management of Barrett's oesophagus.," *Gut* **63**(1), 7–42 (2014) [doi:10.1136/gutjnl-2013-305372].
- 150 8. D. J. Waterhouse et al., "Emerging optical methods for endoscopic surveillance of Barrett's oesophagus," *Lancet Gastroenterol. Hepatol.* **3**(5), 349–362, Elsevier Ltd (2018) [doi:10.1016/S2468-1253(18)30030-X].
9. H. Brown et al., "Scoping the future: An evaluation of endoscopy capacity across the NHS in England" (2015).
10. I. J. Bigio and S. Fantini, *Quantitative Biomedical Optics*, Cambridge University Press (2016) [doi:10.1017/CBO9781139029797].
- 155 11. M. I. Auvinen et al., "Incipient angiogenesis in Barrett's epithelium and lymphangiogenesis in Barrett's adenocarcinoma," *J. Clin. Oncol.* **20**(13), 2971–2979 (2002) [doi:10.1200/JCO.2002.09.011].
12. D. J. Waterhouse et al., "Spectral endoscopy enhances contrast for neoplasia in surveillance of Barrett's esophagus," *Cancer Res.* **81**, 3415–3425 (2021).
- 160 13. G. Lu and B. Fei, "Medical hyperspectral imaging: a review.," *J. Biomed. Opt.* **19**(1), 10901 (2014) [doi:10.1117/1.JBO.19.1.10901].
14. M. A. Calin et al., "Hyperspectral Imaging in the Medical Field: Present and Future," *Appl. Spectrosc.*

Rev. **49**(6), 435–447 (2014) [doi:10.1080/05704928.2013.838678].

- 165 15. Y. Imamoto and Y. Shichida, “Cone visual pigments,” Biochim. Biophys. Acta - Bioenerg. **1837**(5), 664–
673, Elsevier B.V. (2014) [doi:10.1016/j.bbabi.2013.08.009].
- 170 16. K. Gono, “Narrow band imaging: Technology basis and research and development history,” Clin. Endosc. **48**(6), 476–480 (2015) [doi:10.5946/ce.2015.48.6.476].
- 175 17. A. J. de Groof et al., “Blue-light imaging has an additional value to white-light endoscopy in visualization
of early Barrett’s neoplasia: an international multicenter cohort study,” Gastrointest. Endosc. **89**(4), 749–
758, American Society for Gastrointestinal Endoscopy (2019) [doi:10.1016/j.gie.2018.10.046].
- 180 18. A. S. Luthman et al., “Bimodal reflectance and fluorescence multispectral endoscopy based on spectrally
resolving detector arrays,” J. Biomed. Opt. **24**(03), 031009 (2018) [doi:10.11117/1.jbo.24.3.031009].
- 185 19. Y. Fawzy, S. Lam, and H. Zeng, “Rapid multispectral endoscopic imaging system for near real-time
mapping of the mucosa blood supply in the lung,” Biomed. Opt. Express **6**(8), 2980–2990 (2015)
[doi:10.1364/BOE.6.002980].
20. R. T. Kester et al., “Real-time snapshot hyperspectral imaging endoscope,” J. Biomed. Opt. **16**(5), 056005
(2011) [doi:10.11117/1.3574756].
21. T. Saito and H. Yamaguchi, “Optical imaging of hemoglobin oxygen saturation using a small number of
spectral images for endoscopic application,” J. Biomed. Opt. **20**(12), 126011 (2015)
[doi:10.11117/1.JBO.20.12.126011].
22. W. R. Johnson et al., “Snapshot hyperspectral imaging in ophthalmology,” J. Biomed. Opt. **12**(1), 014036
(2007) [doi:10.11117/1.2434950].
23. M. Mori et al., “Intraoperative visualization of cerebral oxygenation using hyperspectral image data: a two-
dimensional mapping method,” Int. J. Comput. Assist. Radiol. Surg. **9**(6), 1059–1072 (2014)
[doi:10.1007/s11548-014-0989-9].
24. L. E. MacKenzie et al., “In vivo oximetry of human bulbar conjunctival and episcleral microvasculature
using snapshot multispectral imaging,” Exp. Eye Res. **149**, 48–58, Elsevier Ltd (2016)
[doi:10.1016/j.exer.2016.06.008].
25. J. Pichette et al., “Intraoperative video-rate hemodynamic response assessment in human cortex using
snapshot hyperspectral optical imaging,” Neurophotonics **3**(4), 045003 (2016)

[doi:10.1117/1.nph.3.4.045003].

26. K. Iwaki et al., “A Novel Hyperspectral Imaging System for Intraoperative Prediction of Cerebral Hyperperfusion Syndrome after Superficial Temporal Artery-Middle Cerebral Artery Anastomosis in Patients with Moyamoya Disease,” *Cerebrovasc. Dis.* **8582**, 208–215 (2021) [doi:10.1159/000513289].
- 195 27. S. E. Martinez-Herrera et al., “Multispectral Endoscopy to Identify Precancerous Lesions in Gastric Mucosa,” 43–51, Springer, Cham (2014) [doi:10.1007/978-3-319-07998-1_6].
28. S. J. Leavesley et al., “Hyperspectral imaging fluorescence excitation scanning for colon cancer detection,” *J. Biomed. Opt.* **21**(10), 104003 (2016) [doi:10.1117/1.JBO.21.10.104003].
- 500 29. Z. Han et al., “*In vivo* use of hyperspectral imaging to develop a noncontact endoscopic diagnosis support system for malignant colorectal tumors,” *J. Biomed. Opt.* **21**(1), 016001 (2016) [doi:10.1117/1.JBO.21.1.016001].
30. R. Kumashiro et al., “An integrated endoscopic system based on optical imaging and hyper spectral data analysis for colorectal cancer detection,” *Anticancer Res.* **3932**, 3925–3932 (2016).
- 505 31. J. Shapey et al., “Intraoperative multispectral and hyperspectral label-free imaging: A systematic review of *in vivo* clinical studies,” *J. Biophotonics* **12**(9) (2019) [doi:10.1002/jbio.201800455].
32. E. Kho et al., “Hyperspectral imaging for resection margin assessment during cancer surgery,” *Clin. Cancer Res.* **25**(12), 3572–3580 (2019) [doi:10.1158/1078-0432.CCR-18-2089].
33. Z. Liu et al., “Automated tongue segmentation in hyperspectral images for medicine.,” *Appl. Opt.* **46**(34), 8328–8334 (2007) [doi:10.1364/AO.46.008328].
- 510 34. H. Akbari et al., “Wavelet-based compression and segmentation of hyperspectral images in surgery,” *Lect. Notes Comput. Sci. (including Subser. Lect. Notes Artif. Intell. Lect. Notes Bioinformatics)* **5128**, 142–149 (2008) [doi:10.1007/978-3-540-79982-5_16].
35. N. Hagen and M. W. Kudenov, “Review of snapshot spectral imaging technologies,” *Opt. Eng.* **52**(9), 090901 (2013) [doi:10.1117/1.OE.52.9.090901].
- 515 36. X. Gu et al., “Image enhancement based on *in vivo* hyperspectral gastroscopic images: a case study,” *J. Biomed. Opt.* **21**(10), 101412 (2016) [doi:10.1117/1.JBO.21.10.101412].
37. R. Leitner et al., “Multi-spectral video endoscopy system for the detection of cancerous tissue,” *Pattern Recognit. Lett.* **34**(1), 85–93, Elsevier B.V. (2013) [doi:10.1016/j.patrec.2012.07.020].

38. C. Yang et al., “Scanning Fiber Endoscope with multiple fluorescence-reflectance imaging channels for
520 guiding biopsy,” 89360R (2014) [doi:10.1117/12.2038544].
39. C. M. Lee et al., “Scanning fiber endoscopy with highly flexible, 1 mm catheterscopes for wide-field, full-
color imaging,” *J. Biophotonics* **3**(5–6), 385–407 (2010) [doi:10.1002/jbio.200900087].
40. T. H. Tate et al., “Ultraminiature optical design for multispectral fluorescence imaging endoscopes,” *J.
Biomed. Opt.* **22**(3), 036013 (2017) [doi:10.1117/1.JBO.22.3.036013].
- 525 41. A. S. Luthman et al., “Hyperspectral fluorescence imaging with multi wavelength LED excitation,” 6 April
2016, 971111, International Society for Optics and Photonics [doi:10.1117/12.2210855].
42. P. J. Lapray et al., “Multispectral filter arrays: Recent advances and practical implementation,” *Sensors*
14(11), 21626–21659 (2014) [doi:10.3390/s141121626].
43. S. Saxe et al., “Advances in miniaturized spectral sensors,” *Proc. SPIE* **10657**(1060570B) (2018)
530 [doi:10.1117/12.2304019].
44. D. J. Waterhouse et al., “A roadmap for the clinical implementation of optical-imaging biomarkers,” *Nat.
Biomed. Eng.* **3**(5), 339–353 (2019) [doi:10.1038/s41551-019-0392-5].
45. D. J. Waterhouse et al., “Quantitative evaluation of comb- structure correction methods for multispectral
fibrescopic imaging,” 1–14 (2018) [doi:10.1038/s41598-018-36088-7].
- 535 46. E. L. Bird-Lieberman et al., “Molecular imaging using fluorescent lectins permits rapid endoscopic
identification of dysplasia in Barrett’s esophagus,” *Nat. Med.* **18**(2), 315–321 (2012)
[doi:10.1038/nm.2616].
47. A. A. Neves et al., “Detection of early neoplasia in Barrett ’ s esophagus using lectin-based near-infrared
imaging : an ex vivo study on human tissue,” *Endoscopy* **50**(6), 618–625 (2018).
- 540 48. M. D. Pietro et al., “The combination of autofluorescence endoscopy and molecular biomarkers is a novel
diagnostic tool for dysplasia in Barrett’s oesophagus,” *Gut* **64**(1), 49–56 (2015) [doi:10.1136/gutjnl-2013-
305975].
49. M. F. Dixon, “Gastrointestinal epithelial neoplasia: Vienna revisited,” *Gut* **51**, 130–131 (2002)
[doi:10.1136/gut.51.1.130].
- 545 50. C. M. Bishop, *Pattern Recognition and Machine Learning*, Springer.
51. K. Gono et al., “Appearance of enhanced tissue features in narrow-band endoscopic imaging.,” *J. Biomed.*

Opt. **9**(3), 568–577, International Society for Optics and Photonics (2004) [doi:10.1117/1.1695563].

52. N. G. Terry et al., “Detection of dysplasia in Barrett’s esophagus with in vivo depth-resolved nuclear morphology measurements,” *Gastroenterology* **140**(1), 42–50 (2011) [doi:10.1053/j.gastro.2010.09.008].
- 550 53. L. B. Lovat et al., “Elastic scattering spectroscopy accurately detects high grade dysplasia and cancer in Barrett’s oesophagus,” *Gut* **55**(8), 1078–1083 (2006) [doi:10.1136/gut.2005.081497].
54. P. Sharma et al., “The American Society for Gastrointestinal Endoscopy PIVI (Preservation and Incorporation of Valuable Endoscopic Innovations) on imaging in Barrett’s Esophagus,” *Gastrointest. Endosc.* **76**(2), 252–254 (2012) [doi:10.1016/j.gie.2012.05.007].
- 555 55. N. Thosani et al., “ASGE Technology Committee systematic review and meta-analysis assessing the ASGE Preservation and Incorporation of Valuable Endoscopic Innovations thresholds for adopting real-time imaging-assisted endoscopic targeted biopsy during endoscopic surveillance,” *Gastrointest. Endosc.* **83**(4), 684–698, Elsevier, Inc. (2016) [doi:10.1016/j.gie.2016.01.007].
56. C. Williams et al., “Grayscale-to-Color: Scalable Fabrication of Custom Multispectral Filter Arrays,” *ACS Photonics* **6**(12), 3132–3141 (2019) [doi:10.1021/acsphotonics.9b01196].
- 560 57. Q. Chen et al., “Nanophotonic Image Sensors,” *Small* **12**(36), 4922–4935 (2016) [doi:10.1002/smll.201600528].
58. W. Sun and Q. Du, “Hyperspectral band selection: A review,” *IEEE Geosci. Remote Sens. Mag.* **7**(2), 118–139, IEEE (2019) [doi:10.1109/MGRS.2019.2911100].


565

Table**Table 1 | Summary of the collected image cubes and biopsies for matched regions**

Trial Number	Barrett's Length (C = Circumferential, M = Maximum Extent) / cm	Location / cm	Location / o'clock	Initial Label During Endoscopy	Tissue Acquisition	Diagnosis from Histopathology	Number of Matched Image Cubes
3	C0M2	37	8	Suspicious	EMR x 1	NDBE	12
		37	4	Control	Biopsy x 1	NDBE	11
4	C4M6	36	6	Control	Biopsy x 1	NDBE	60
5	C5M7	31	9	Control	Biopsy x 1	NDBE	28
6	C11M14	31	9	Control	Biopsy x 1	NDBE	6
		28	6	Control	Biopsy x 1	NDBE	9
7	C11M12	35	9	Control	Biopsy x 2	NDBE	8
		32	5	Control	Biopsy x 2	NDBE	7
8	C6M7	32	12	Control	Biopsy x 1	NDBE	32
		30	6	Control	Biopsy x 1	NDBE	4
9	C5M7	34	3	Suspicious	EMR x 1	IMC	9
		33	3	Suspicious	EMR x 1	IMC	15
		30	9	Control	Biopsy x 1	NDBE	5
10	C14M14	32	10	Suspicious	Biopsy x 2	HGD	8
		24	10	Control	Biopsy x 1	NDBE	7
11	C2M5	35	12	Suspicious	EMR x 1	HGD	8
		36	6	Control	Biopsy x 1	NDBE	15
12	C2M4	41	6	Suspicious	EMR x 1	LGD	30
		39	8	Control	None	NA	5
		39	6	Control	Biopsy x 1	LGD	3
14	C0M3	36	3	Suspicious	Biopsy x 2	NDBE	8
		38	3	Control	Biopsy x 1	NDBE	7
15	C3M4	35–38	9	Suspicious	EMR x 4	IMC	11
		37	3	Control	Biopsy x 1	NDBE	8
16	C0M4	40	11	Suspicious	Biopsy x 1	IMC	7
		39	3	Control	Biopsy x 1	NDBE	4
17	C0M2	37	1	Suspicious	Biopsy x 2	NDBE	7
18	C5M7	26	12	Suspicious	EMR x 2	HGD	134
		25	9	Control	Biopsy x 1	NDBE	95
		26	3	Suspicious	EMR x 1	HGD	7


EMR, endoscopic mucosal resection; HGD, high grade dysplasia; IMC, intramucosal carcinoma; LGD, low grade dysplasia; NDBE, non-dysplastic Barrett's esophagus; NR, not reported.

580 **Figures**

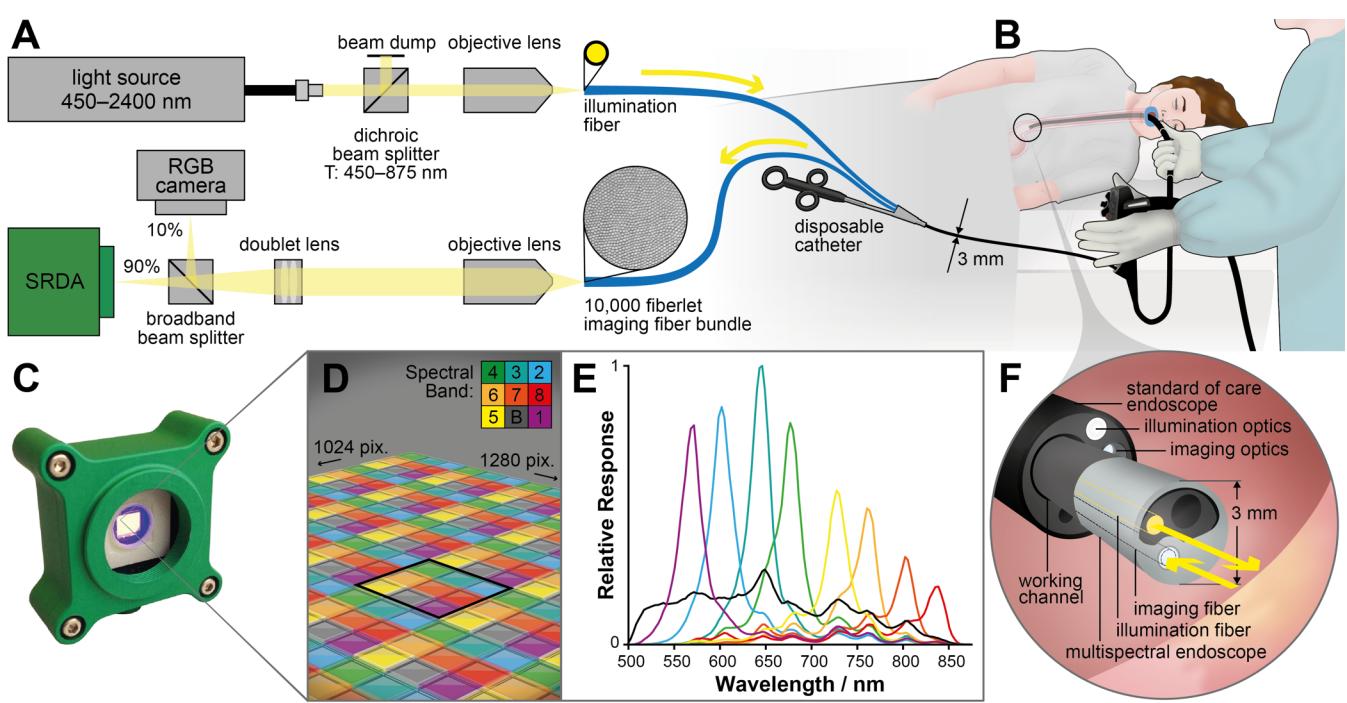

580 **Figure 1 | A compact snapshot multispectral endoscope for esophageal imaging.**

(A) Light from a broadband supercontinuum light source enters the patient via a single illumination fiber. Reflected light is returned via a 10,000 fiberlet imaging bundle. (B) The ‘babyscope’ enters the esophagus via the working channel of a standard of care endoscope. (C) Light is detected by a spectrally resolved detector array (SRDA). (D) This includes a 3 x 3 mosaic of color filters, 8 narrow bands and 1 broad band (B) deposited directly on the sensor pixel. (E) The spectral response of the detection channel of the multispectral endoscope is shown. (F) Light is delivered to the esophageal lumen via the ‘babyscope’ illumination fiber and diffusely reflected light is collected by the imaging fiber bundle.

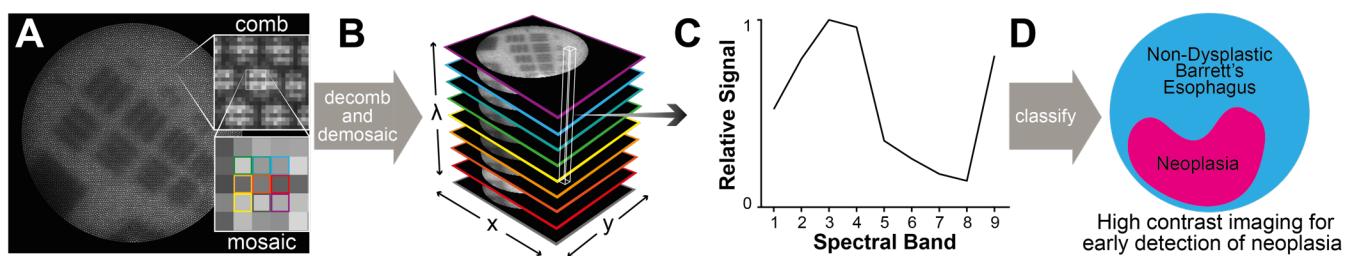

590 **Figure 2 | Data processing for snapshot multispectral endoscopy.**

(A) Raw collected data contains comb and mosaic artefacts from the imaging fiber and SRDA respectively. (B) These are removed by a demosaicing and decombining algorithm to produce a spectral data cube. (C) For a given pixel in the image cube, a 9-band per-pixel spectrum can be determined. (D) By using these per-pixel spectra, machine-learning-based classification algorithms can interpret the image cube to generate a classification map, thus helping to guide the endoscopist.

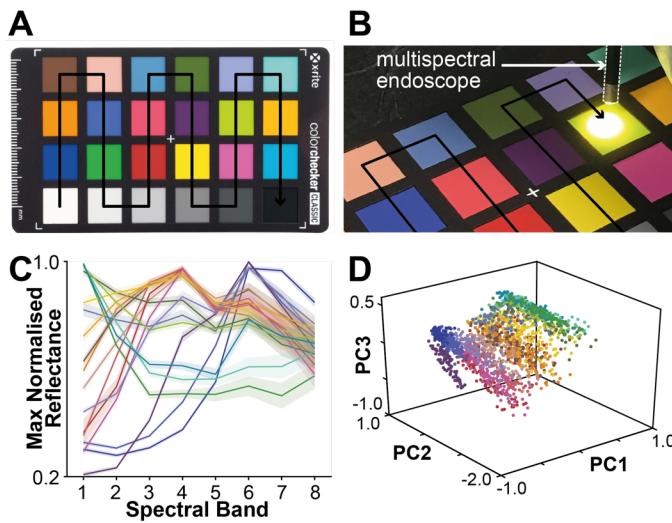


Figure 3 | Color chart imaging

(A) A Macbeth color chart was used to validate the multispectral endoscope. (B) Handheld imaging of the Macbeth color chart took place prior to 4 of the *in vivo* trials. (C) The mean per-pixel spectra for each color on the Macbeth color chart are distinct, but overlap within their variation, Shaded region shown is standard deviation / 5 for clarity. (D) Principle component analysis show clustering of the per-pixel spectra by color, but also show the overlap of similar colors.

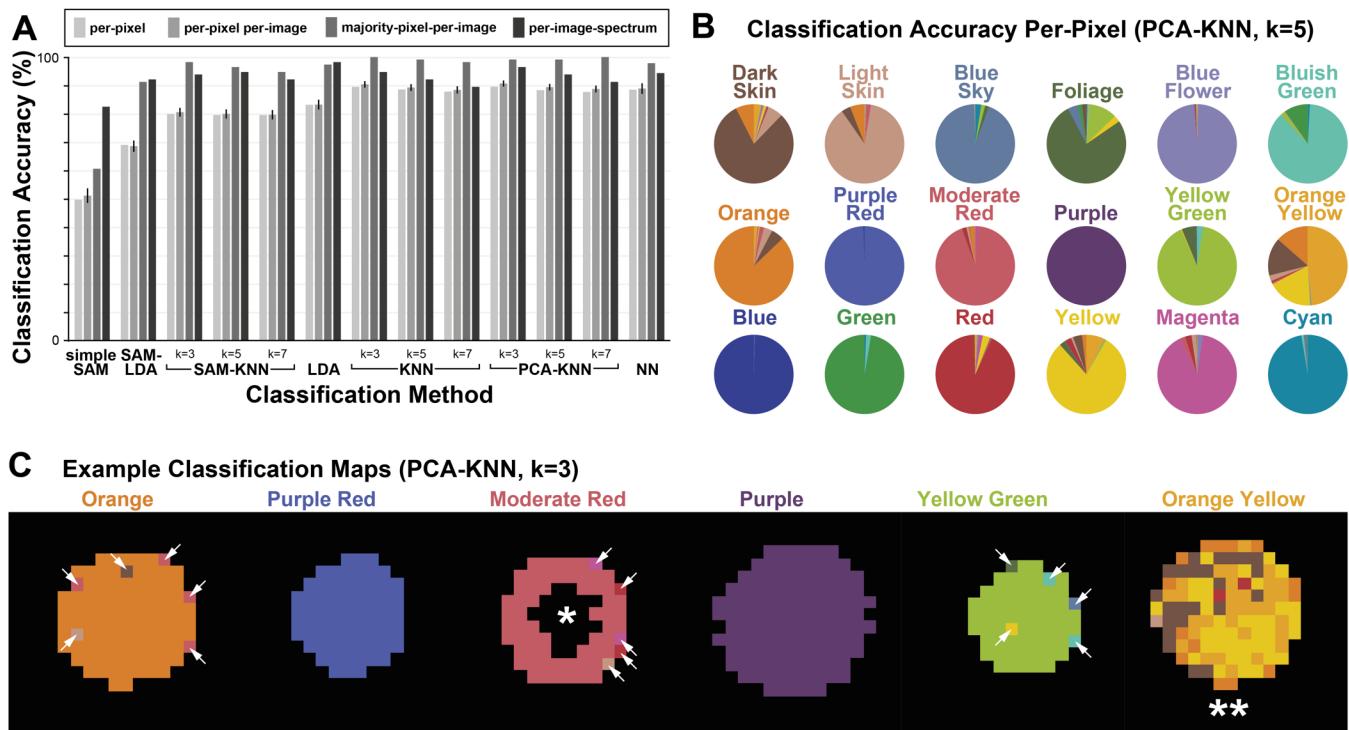


Figure 4 | Machine learning enables classification of multispectral images of color chart.

(A) Seven classification approaches were compared for classification of color chart image cubes. The best classification approach was PCA-KNN. (B) Per-pixel accuracies are shown as pie charts for each color in the Macbeth color chart. (C)

Example classification maps are shown for 40-pixel x 32-pixel x 9-band image cubes of the middle color row of the Macbeth color chart. White arrows highlight misclassified pixels, which often lie close to the edge of the illuminated region. * The dark hole in the center of the ‘moderate red’ image is a region of specular reflection. ** Many of the ‘orange yellow’ pixels are misclassified but are of a similar shade to the correct ‘orange yellow’ color.


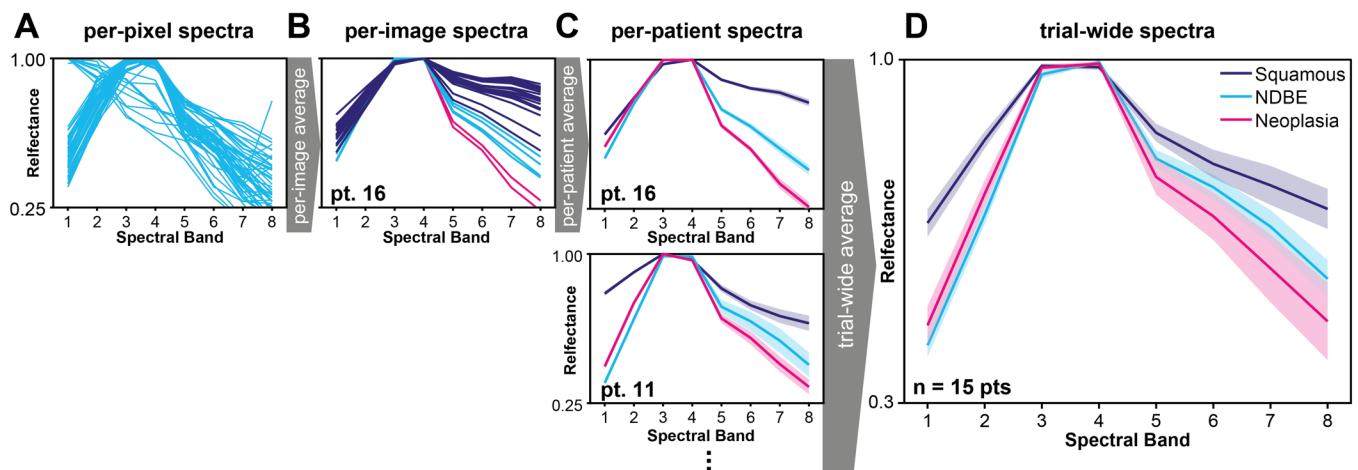


Figure 5 | Spectra show promising differences between tissue types.

(A) Per-pixel spectra for a single image of NDBE in patient 16. (B) All per-image spectra for patient 16. (C) Per-patient spectra for patient 16 and patient 11 are shown. The shaded region is the standard error from the standard deviation of per-image spectra. (D) The trial-wide spectra. The shaded region is the standard error from the standard deviation across per-patient spectra.

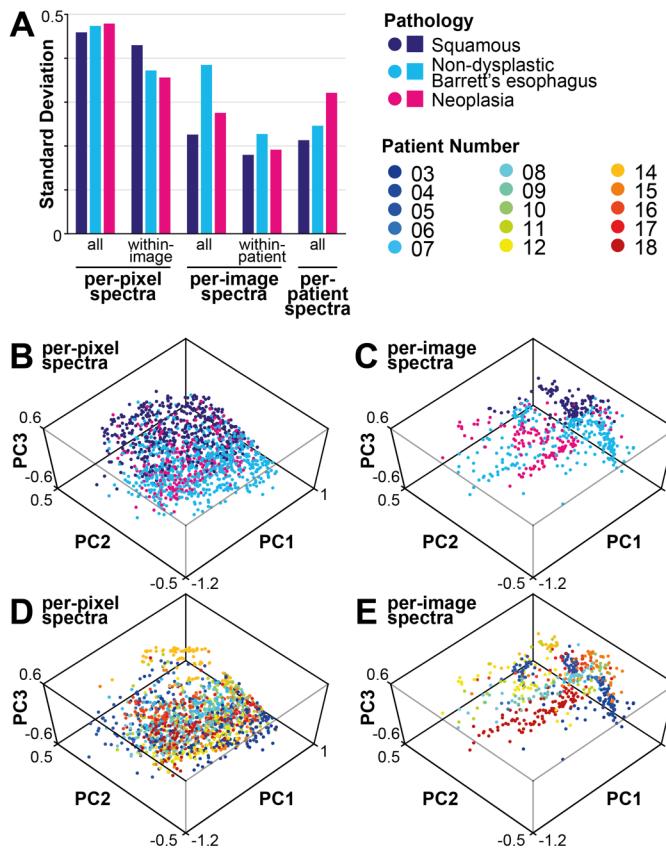

520 **Figure 6 | Spectra show considerable variance between patients.**

(A) The standard deviation is shown for per-pixel spectra, per-image spectra and per-patient spectra for each pathology class.

(B) Principle component analysis (PCA) for per-pixel spectra show clustering by pathology but with considerable overlap. (C)

525 PCA of per-image spectra shows a more defined clustering per-pathology. Both per-pixel spectra (D) and per-image spectra

(E) show visible clustering by patient, making clear the inter-patient heterogeneity in the dataset.

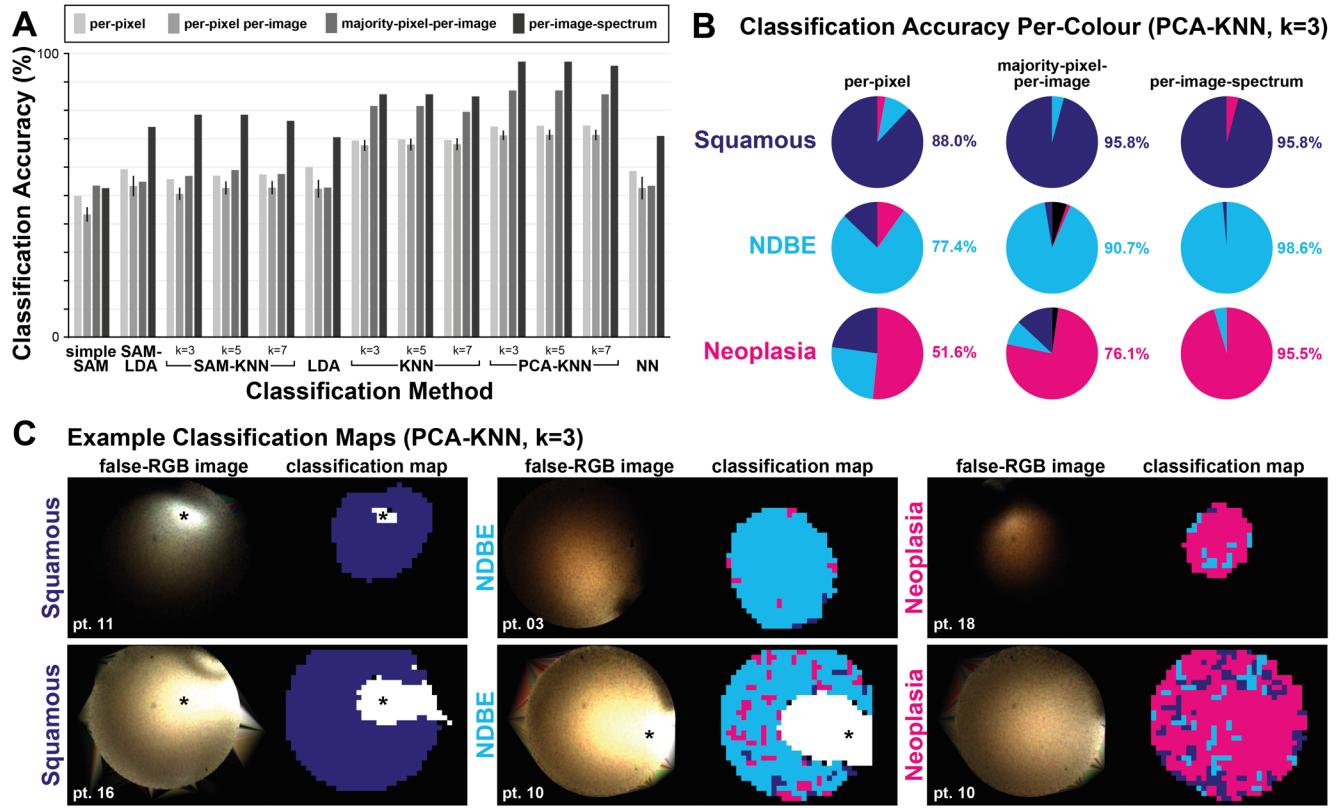


Figure 7 | Snapshot multispectral endoscopy shows promising accuracy for *in vivo* tissue classification.

(A) Seven approaches were compared for tissue classification. (B) The best classification approach was PCA-KNN with $k = 3$.

530 Per-pixel, majority-pixel-per-image and per-image-spectrum accuracies are shown for each pathology. Black sectors represent images where majority pixel decision could not be reached. (C) Example classification maps of 40-pixel x 32-pixel x 9-band image cubes are shown for each pathology alongside the matched false-RGB image generated by assigning bands 2, 3 and broadband to R, G and B colors respectively. * Specular reflections are excluded from classification and marked as white in the classification maps.

