



Indirect photo-electrochemical detection of carbohydrates with Pt@g-C₃N₄ immobilised into a polymer of intrinsic microporosity (PIM-1) and attached to a palladium hydrogen capture membrane

Yuanzhu Zhao^a, Joshua Dobson^a, Catajina Harabajiu^a, Elena Madrid^a, Tinakorn Kanyanee^{a,b,c}, Catherine Lyall^{a,d}, Shaun Reeksting^{a,d}, Mariolino Carta^e, Neil B. McKeown^f, Laura Torrente-Murciano^g, Kate Black^h, Frank Marken^{a,*}

^a Department of Chemistry, University of Bath, Claverton Down, Bath BA2 7AY, UK

^b Department of Chemistry, Faculty of Science, Chiang Mai University, Chiang Mai 50200, Thailand

^c Center of Excellence in Materials Science and Technology, Chiang Mai University, Chiang Mai 50200, Thailand

^d Material & Chemical Characterisation Facility MC², University of Bath, Bath BA2 7AY, UK

^e Department of Chemistry, Swansea University, College of Science, Grove Building, Singleton Park, Swansea SA2 8PP, UK

^f School of Chemistry, University of Edinburgh, Joseph Black Building, West Mains Road, Edinburgh, Scotland EH9 3JJ, UK

^g Department of Chemical Engineering and Biotechnology, University of Cambridge, Philippa Fawcett Drive, Cambridge CB3 0AS, UK

^h University of Liverpool, School of Engineering, Liverpool L69 3BX, UK

ARTICLE INFO

Article history:

Received 7 January 2020

Received in revised form 4 March 2020

Accepted 6 March 2020

Available online 7 March 2020

Keywords:

Carbohydrate

Hydrogen

Photocatalysis

Polymer

Reaction layer

Sensor

ABSTRACT

An “indirect” photo-electrochemical sensor is presented for the measurement of a mixture of analytes including reducing sugars (e.g. glucose, fructose) and non-reducing sugars (e.g. sucrose, trehalose). Its innovation relies on the use of a palladium film creating a two-compartment cell to separate the electrochemical and the photocatalytic processes. In this original way, the electrochemical detection is separated from the potential complex matrix of the analyte (i.e. colloids, salts, additives, etc.). Hydrogen is generated in the photocatalytic compartment by a Pt@g-C₃N₄ photocatalyst embedded into a hydrogen capture material composed of a polymer of intrinsic microporosity (PIM-1). The immobilised photocatalyst is deposited onto a thin palladium membrane, which allows rapid pure hydrogen diffusion, which is then monitored by chronopotentiometry (zero current) response in the electrochemical compartment. The concept is demonstrated herein for the analysis of sugar content in commercial soft drinks. There is no requirement for the analyte to be conducting with electrolyte or buffered. In this way, samples (biological or not) can be simply monitored by their exposition to blue LED light, opening the door to additional energy conversion and waste-to-energy applications.

© 2020 The Authors. Published by Elsevier B.V. This is an open access article under the CC BY license (<http://creativecommons.org/licenses/by/4.0/>).

1. Introduction


Photo-electroanalytical sensing [1,2] and photo-bioelectro-analytical processes [3] provide a way to detect analytes under light-activated conditions with applied current/potential and illumination (continuous or pulsed [4,5]). There have been several cases of photo-electroanalytical procedures reported previously, for example for glucose detection [6], for miRNA [7], for mercury [8], and for ascorbate [9].

In this paper, a palladium film membrane cell is employed to separate the electrochemical compartment (see Schematic 1) from the photo-catalysis compartment. This separation allows any type

of analytical sample, independent of chemical nature or conductivity, to be studied without direct interference during the electrochemical detection. The palladium membrane purifies the hydrogen before detection and stops the direct interaction of sample and electrode. The process relies on the well-known Pt@g-C₃N₄ photocatalyst [10,11,12] and is based on a sequence of reaction steps. First, the excitation of Pt@g-C₃N₄ (Eq. (1)) is followed by a charge separation step enhanced by the platinum deposit [13] (Eq. (2)). Next, the photo-generated hole can be captured either by water (to give oxygen, Eq. (3)) or by a quencher such as glucose (to give oxidation products, Eq. (4)). The remaining negative charge accumulates on the nano-platinum cocatalyst (here typically 2.5 nm diameter [14]), which results in the formation of hydrogen (Eq. (5)) that then diffuses to/across the palladium membrane. After crossing the membrane, the electrochemical oxidation of





* Corresponding author.

E-mail address: f.marken@bath.ac.uk (F. Marken).

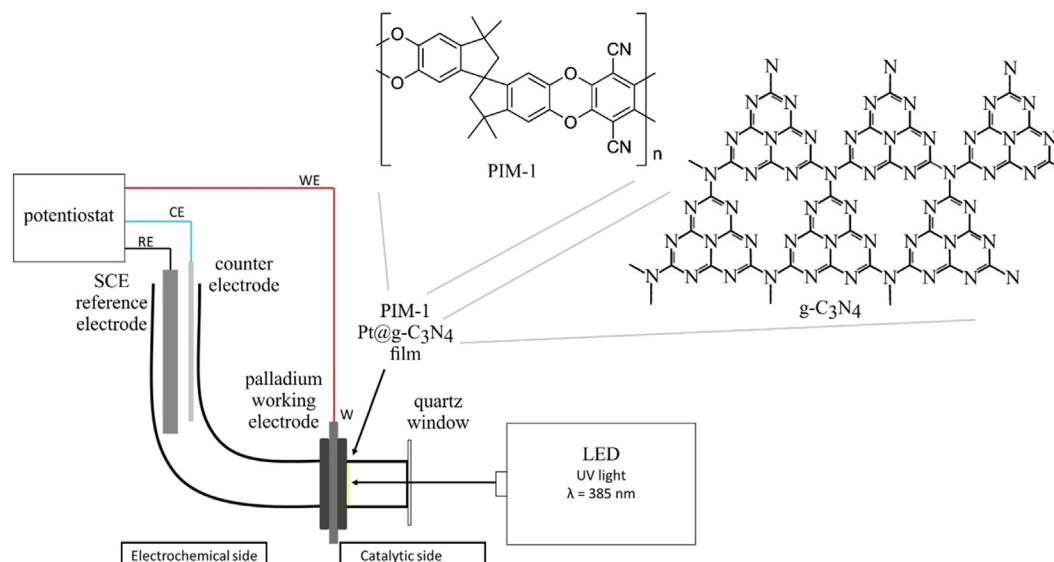

Schematic 1. Schematic illustration of an experimental system with a palladium film (25 μm thickness; optically dense), an electrochemical compartment with counter, reference, and working electrode immersed in aqueous 10 mM HCl, and a photo-catalysis compartment (where analyte is placed) with quartz window, optical path length 15 mm, 385 nm wave length, approximately 100 mW cm^{-2} LED light source.

hydrogen to protons (Eq. (6)) is responsible for the establishment of a new equilibrium potential (in competition with reactions due to ambient oxygen). This sequence of reaction steps is oversimplified due to ambient oxygen introducing further complexity on both sides of the palladium membrane (*vide infra*).



The immobilisation of the photocatalyst onto the palladium membrane surface can be achieved with a polymer of intrinsic microporosity. The use of a polymer of intrinsic microporosity (or PIM) is not only a simple scaffold to hold the catalyst without binding to the photocatalyst surface, but it is also beneficial, based on recent progress, in controlling the transport of gas molecules (under triphasic conditions) at electrode surfaces [15]. PIMs have been developed a decade ago [16] as a novel class of glassy (molecularly rigid) porous materials with excellent processability. Recently, these materials have emerged as useful components in electrochemical processes [17] due to the ability to stabilise surfaces, immobilise catalysts [18], and to capture gases such as hydrogen under “triphasic” conditions in the presence of aqueous electrolytes [19]. PIM-1 offers a surface area (BET) of typically $750 \text{ m}^2 \text{ g}^{-1}$ [20] and pores of around 1–2 nm [21].

In this report, exploratory data are presented to demonstrate the concept of an “indirect” carbohydrate sensor, based on an indirect electrochemical process (*via* palladium membrane) and driven by blue light ($\lambda = 385 \text{ nm}$) in a photo-catalytic reaction. The $\text{Pt@g-C}_3\text{N}_4$ photocatalyst is employed in conjunction with the hydrogen capturing PIM-1 polymer of intrinsic microporosity. Different types of carbohydrates (reducing and non-reducing) are shown to pro-

duce detectable photoresponses. Potential for application of “indirect sensing” is demonstrated with commercial softdrinks.

2. Experimental

2.1. Reagents

All chemicals were purchased from Sigma-Aldrich and used without any further purification. Palladium membrane (0.025 mm thickness, 99.95% purity, light tested) was purchased from Goodfellow Ltd. PIM-1 was prepared following a literature procedure [22]. Commercial softdrinks (a glucose-containing soft-drink “Innocent Coconut Water” (Innocent UK) and a sweetener-containing softdrink “Oasis Aquashock Chilled Cherry” (Coca Cola UK)) were bought from a local supermarket. Deionized water ($18.2 \text{ M}\Omega \text{ cm}$ at 20°C obtained from a CE Instruments Ltd. water purification system) was used to prepare electrolyte solutions. All experiments are conducted in an ambient environment ($T = 22 \pm 2^\circ \text{C}$).

2.2. Instrumentation

Electrochemical measurements were conducted with a potentiostat system ($\mu\text{AUTOLAB III}$, Metrohm, Herisau, Switzerland). GPES software was used to record the data. A KCl-saturated calomel electrode (SCE) was used as the reference electrode together with a platinum wire as the counter electrode. Transmission electron microscopy (TEM) images for $\text{Pt@g-C}_3\text{N}_4$ materials were captured with a JEOL JSM-2010Plus (JEOL U.K. Ltd, Welwyn Garden City, UK). An LED light source wavelength 385 nm was employed (Thorlabs, Inc., M385LP1). ^1H NMR spectra was recorded on a Bruker 500 MHz spectrometer. Mass spectrometry analyses were performed on an Automated Agilent QTOF (Walkup) used with HPLC (4 chromatography columns) and variable wavelength detector (VWD). LC-MS analyses were performed using an Agilent QTOF 6545 with Jetstream ESI spray source coupled to an Agilent 1260 Infinity II Quat pump HPLC with 1260 autosampler, column oven compartment and variable wavelength detector (VWD).

2.3. Procedures

Synthesis of Pt@g-C₃N₄. First, melamine (Sigma-Aldrich, 99% purity) was added into a ceramic boat with lid, which was then placed into the centre of an Elite horizontal tube furnace (TSH12/65/550) and heated to 500 °C for three hours. After cooling overnight, the final g-C₃N₄ was obtained as pale-yellow powder. Next, potassium hexachloroplatinate(IV) (K₂PtCl₆) (purchased from Sigma-Aldrich, >99.9% purity) (40 mg) and 0.4 g of the synthesised g-C₃N₄ were added into 25 mL of saturated sodium oxalate solution in a glass vial. In order to deposit platinum nanoparticles (Pt⁰) onto the g-C₃N₄, the reaction mixture was irradiated with blue light ($\lambda = 385$ nm) for 60 h with continuous stirring. Pt@g-C₃N₄ catalyst was finally separated and collected by centrifuging, washing, and drying in an oven.

Immobilisation of photocatalyst into PIM-1. Pt@g-C₃N₄ catalyst was dispersed together with the polymer of intrinsic microporosity (PIM-1) in a chloroform solution. The mixture was ultrasonicated in a water bath for 15 mins before use. Deposits were formed by drop-casting.

Preparation of Pd membrane. A piece of commercial document lamination foil was firstly punctured with a hole with a 2 mm diameter. A Pd foil (0.025 mm thickness, 0.5 cm × 0.5 cm, Goodfellow Ltd.) was then placed between the two pieces of the laminate (see Fig. 1A). A strip of copper film was placed in contact with the Pd foil for electrical connection. The laminate was then sealed with a hot iron to achieve sealing. Fig. 1B and C show schematic drawings of the photocatalyst deposited with a PIM-1 coating and a mixed coating with both photocatalyst and PIM-1. The latter proved to be a more robust methodology and was applied throughout the study. In Fig. 1D TEM images are shown revealing platinum nanoparticles of typically 2.5 nm diameter.

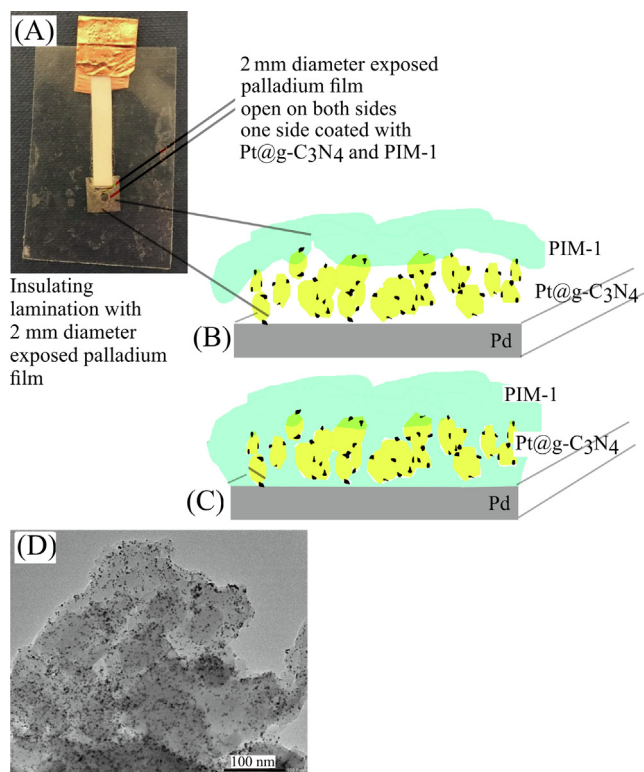


Fig. 1. (A) Photograph of the laminated palladium film exposed with 2 mm diameter holes on both sides. (B) Schematic drawing of Pt@g-C₃N₄ immobilised on palladium and coated with PIM-1. (C) Schematic drawing of Pt@g-C₃N₄ with PIM-1 coated as a single layer. (D) Typical transmission electron micrograph (TEM) for Pt@g-C₃N₄.

3. Results and discussion

3.1. Pt@g-C₃N₄ photopotential responses due to hydrogen from glucose

The production of hydrogen from glucose by the Pt@g-C₃N₄ photocatalyst can be revealed due to rapid hydrogen diffusion through the adjacent palladium film [23]. The diffusion coefficient for hydrogen in palladium has been reported as approximately $3 \times 10^{-11} \text{ m}^2 \text{ s}^{-1}$ at room temperature [24,25] and therefore the response time delay due to hydrogen diffusing through the $L = 25 \mu\text{m}$ membrane will be typically $\tau \approx L^2/D = 20 \text{ s}$. The advantage of the palladium film separating the electrochemical compartment and the photocatalysis compartment (see Schematic 1) is based on the purification of the hydrogen transiting the palladium. In this way it is possible to suppress any interfering redox response from the sample.

Chronoamperometry at zero current was chosen to follow the photoresponse in terms of an equilibrium potential signal. Fig. 2A shows some typical chronoamperometry data traces. Only distilled water (i) does not lead to a significant potential response due to oxygen on both sides of the palladium membrane dominating the redox equilibrium. Trace (ii) shows a slight negative shift, but with a stable equilibrium potential when 0.1 M NaOH is added into

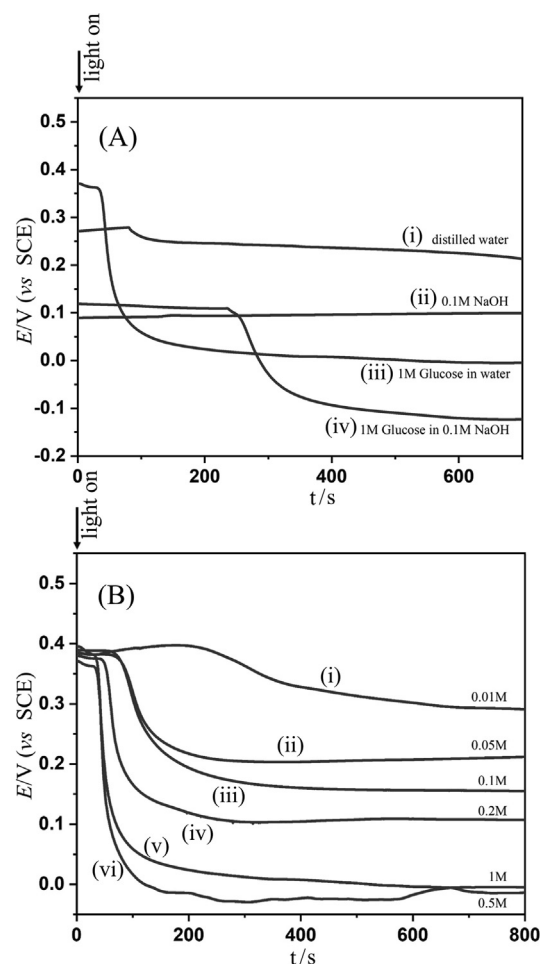


Fig. 2. (A) Chronopotentiometry (zero current) for a palladium film in contact to four different solutions: (i) distilled water, (ii) 0.1 M NaOH, (iii) 1 M glucose in water, and (iv) 1 M glucose in 0.1 M NaOH. Photocatalyst: 60 μg Pt@g-C₃N₄ mixed with 12 μg PIM-1 on a 2 mm diameter Pd membrane area. At time zero the LED is switched on. Electrochemical compartment (see inset) with aqueous 10 mM HCl. (B) Chronopotentiometry (zero current) for glucose in water with (i) 0.01, (ii) 0.05, (iii) 0.1, (iv) 0.2, (v) 0.5, and (vi) 1 M glucose.

the catalysis compartment. The presence of glucose in the aqueous solution makes a significant difference. In both, water with glucose (iii) and 0.1 M NaOH with glucose (iv), a delayed and pronounced shift to negative potentials (0.00 and -0.12 V vs. SCE, respectively) is observed. This shift can be attributed to the photocatalytic hydrogen evolution due to glucose acting as a hole quencher. Perhaps interestingly, the delay is more pronounced in 0.1 M NaOH, but the final potential is also substantially more negative (more hydrogen is produced). The delay is (at least in part) due to the need to locally consume oxygen present on both sides of the palladium membrane (*vide infra*). Due to the complexity of the chemistry of glucose in alkaline media and the additional benefit of not requiring any electrolyte in the photocatalysis compartment, the following experiments were conducted in pure water.

Data in Fig. 2B were obtained with different concentrations of glucose dissolved in water. An amount of $60\text{ }\mu\text{g}$ Pt@g-C₃N₄ photocatalyst was immobilized together with $12\text{ }\mu\text{g}$ PIM-1. A signal can be measured for a concentration as low as 10 mM glucose. However, the delay is substantial (300 s) and the final potential does not significantly shift. When increasing the glucose concentration, the hydrogen response is observed to be faster (within 60 s) and the shift in equilibrium potential is more pronounced. A dependence of the final equilibrium potential on the glucose concentration is observed.

Next, the effect of the PIM-1 polymer is investigated. Fig. 3 shows chronoamperometry (zero current) data obtained for (A) $60\text{ }\mu\text{g}$ Pt@g-C₃N₄ with $24\text{ }\mu\text{g}$ PIM-1 and (B) $60\text{ }\mu\text{g}$ Pt@g-C₃N₄ with no PIM-1. The presence of the polymer of intrinsic microporosity

does affect the behaviour of the photocatalyst. An increase in PIM-1 appears to slow down the photoresponse as well as shifting the final equilibrium potential slightly more positive. This increase and shift is consistent with the additional PIM-1 either slowing diffusional access to the photocatalyst or somewhat lowering the light intensity at the location of the photocatalyst.

In the absence of PIM-1 (see Fig. 3B), the equilibrium potential response is significantly delayed and observed only for very high concentrations of glucose (for less than 0.5 M glucose the process occurs not within 1000 s). This can be explained with the competing fluxes of hydrogen and oxygen to the photocatalyst. Fig. 3D shows a schematic diagram indicating production of hydrogen at the photocatalyst and diffusion of oxygen from outside into the PIM-1 layer. As a microporous polymer, PIM-1 is open to small molecule diffusion, e.g. glucose, protons, water, and to gas diffusion, e.g. hydrogen and oxygen. However, under triphasic conditions transport of oxygen may be slowed down during hydrogen production. Therefore, the PIM-1 material not only provides mechanical stabilisation of the Pt@g-C₃N₄ photocatalyst, but also a protection against oxygen improving the flux of hydrogen into the palladium membrane. The optimum effects are observed with $60\text{ }\mu\text{g}$ Pt@g-C₃N₄ and $12\text{ }\mu\text{g}$ PIM-1.

Data plotted in Fig. 3C shows the effect of PIM-1 when equilibrium potential data is plotted versus glucose concentration. Without PIM-1 present a delayed and dramatic change is observed. With the PIM-1 present, a more gradual change occurs, and this could be useful when analytically detecting glucose or other types of carbohydrates.

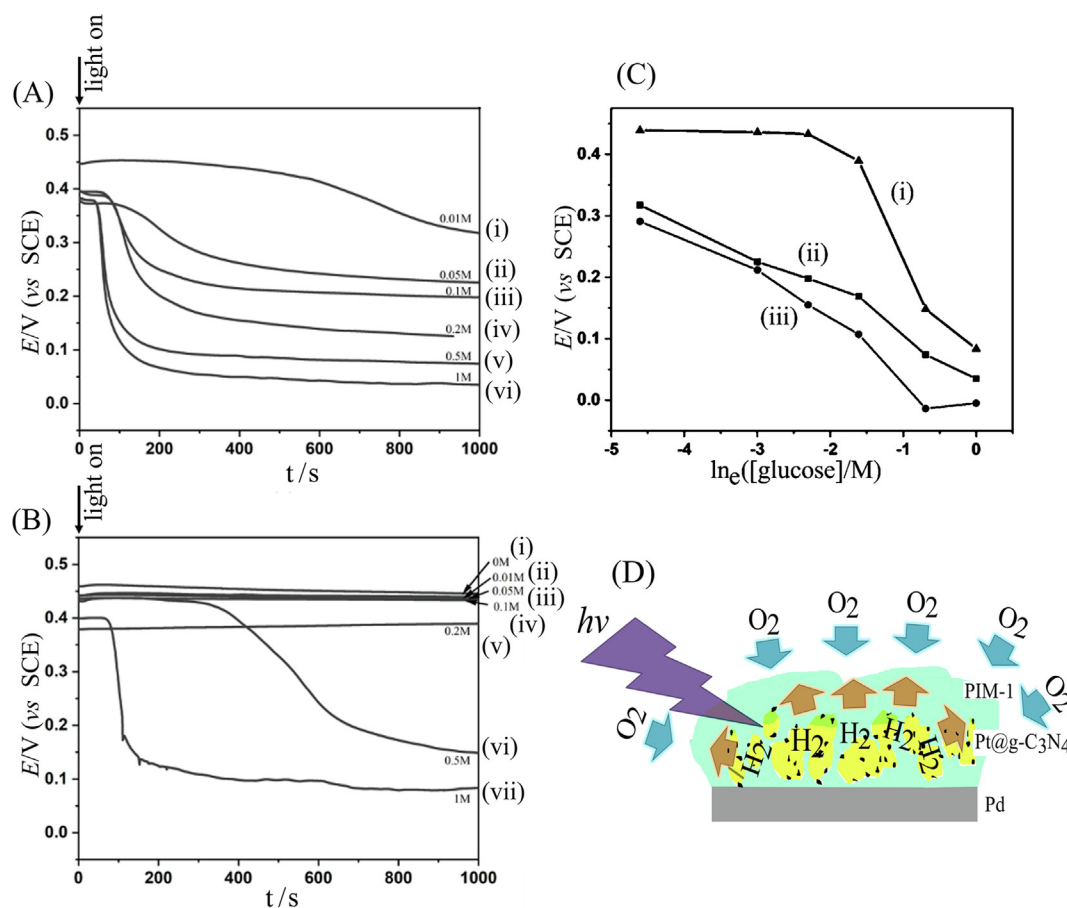


Fig. 3. (A) Chronopotentiometry (zero current) with $60\text{ }\mu\text{g}$ Pt@g-C₃N₄ and $24\text{ }\mu\text{g}$ PIM-1 on palladium in (i) 0.01, (ii) 0.05, (iii) 0.1, (iv) 0.2, (v) 0.5, and (vi) 1 M glucose in water. (B) As before but for only $60\text{ }\mu\text{g}$ Pt@g-C₃N₄ and no PIM-1. (C) Summary plot of end potential (at 1000 s) as a function of glucose concentration in water for (i) no PIM-1, (ii) $24\text{ }\mu\text{g}$ PIM-1, and (iii) $12\text{ }\mu\text{g}$ PIM-1. (D) Schematic drawing of the photocatalytic hydrogen production under a PIM-1 film competing with oxygen ingress.

3.2. Pt@g-C₃N₄ photopotential responses due to hydrogen produced from different carbohydrates

The effects of the carbohydrate molecular structure on the photoreponse was investigated, in particular in view of the behaviour of reducing versus non-reducing sugars. Fig. 4 shows chronoamperometry (zero current) data for glucose, fructose (reducing) as well as sucrose and trehalose (non-reducing). It is clear that both reducing and non-reducing sugars give significant photoreponses. It has previously been suggested that the reaction of the sugar is likely to be associated with its adsorption onto the g-C₃N₄ photocatalyst [14] and therefore holes of high energy (2.7 eV band gap [26]) may be sufficiently energetic to trigger oxidation even for non-reducing carbohydrates. For trehalose (Fig. 4A), the photoreponse is delayed and observed only for concentrations higher than 0.1 M. However, for sucrose (Fig. 4B) only a weak delayed signal is observed. Both glucose (Fig. 2B) and fructose (Fig. 4C) show photoreponses over the complete concentration range. The plot in Fig. 4D summarises and compares the final equilibrium potential data (at 1000 s) for the four types of carbohydrate.

3.3. Pt@g-C₃N₄ photopotential responses due to hydrogen generation from soft drink samples

A potential area of application of the photopotential generation for carbohydrates could be in monitoring of commercial products containing sugars. The palladium membrane is dense separating

the electrochemical compartment from the photocatalysis compartment. Complex samples of any type (even in oils etc.) could be in contact and used to generate photoreponses.

Here, commercial softdrink samples were purchased and tested. Fig. 5A shows the photoreponse for a sugar containing softdrink (see experimental). Filtration was necessary as turbidity affected the measurement. However, in future this could be avoided by shortening the optical path length (here 15 mm). By diluting the sample systematically, a set of data points was recorded. NMR analysis of the product (see supporting information) revealed the presence of an aqueous glucose: fructose: sucrose solution with molar ratio 1: 4.95: 2.42 and with total content of 0.355 g glucose + 1.75 g fructose + 1.3 g sucrose in 100 mL water. An artificial solution of identical composition was used for comparison purposes. Data in Fig. 5B show very similar photoreponses upon dilution. A softdrink with sweetener (no carbohydrates) did not give any significant photoreponse (Fig. 5C). The plot in Fig. 5D shows data for two repeat data sets of the sugar-containing softdrink together with the data for the artificial mixture of sugars showing a good agreement.

It should be noted that these measurements were all performed in the presence of ambient oxygen and this affects the equilibrium potential data (as oxygen will react with hydrogen at the palladium surface). Additional experiments (not shown) with argon de-aeration cause a shift of the final equilibrium to more negative potentials. Argon de-aeration only on the sample side does not speed up the photoreponse but results in a shift in final potential

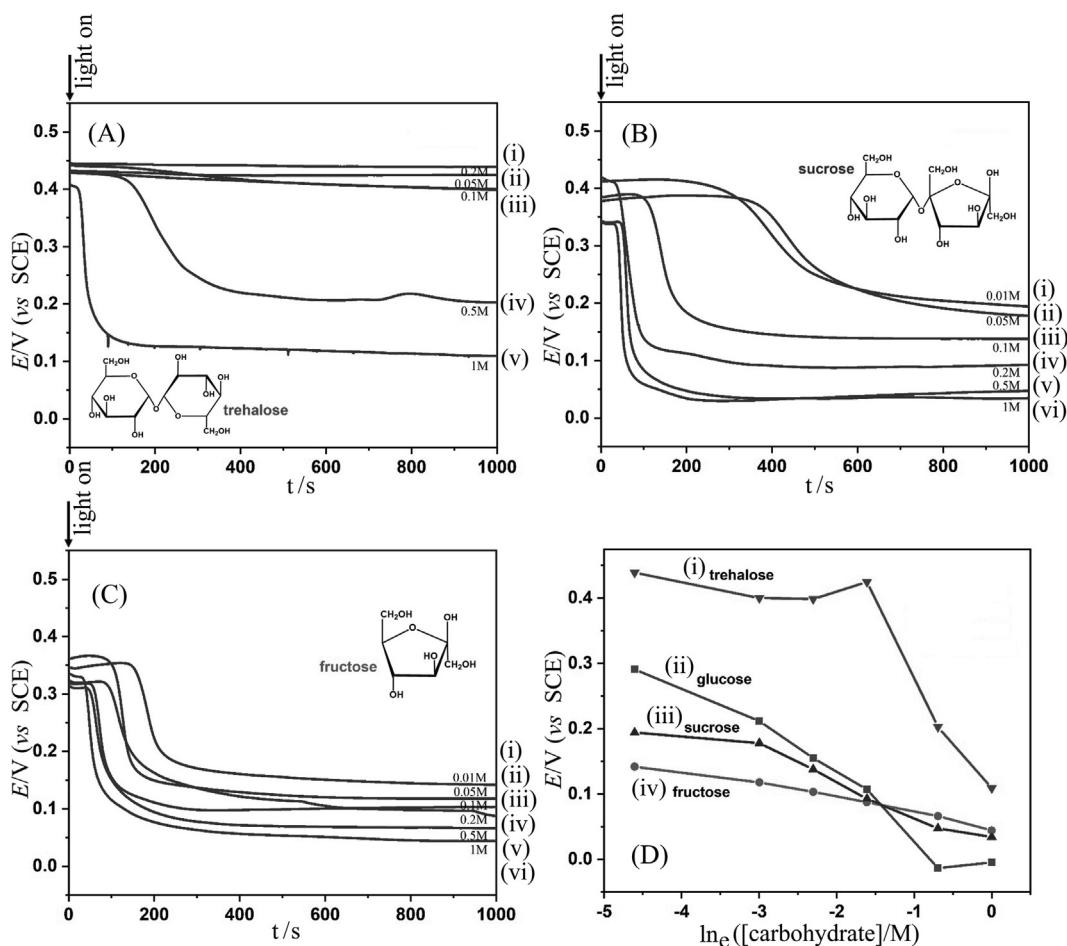


Fig. 4. (A) Chronopotentiometry (zero current) data obtained with 60 μ g Pt@g-C₃N₄ and 12 μ g PIM-1 at a palladium membrane for (i) 0.05, (ii) 0.1, (iii) 0.2, (iv) 0.5, and (v) 1 M trehalose in water. (B) As above but for sucrose. (C) As above but for fructose. (D) Plot of the final equilibrium potential (at 1000 s) versus carbohydrate concentration in water for (i) trehalose, (ii) glucose, (iii) sucrose, and (iv) fructose.

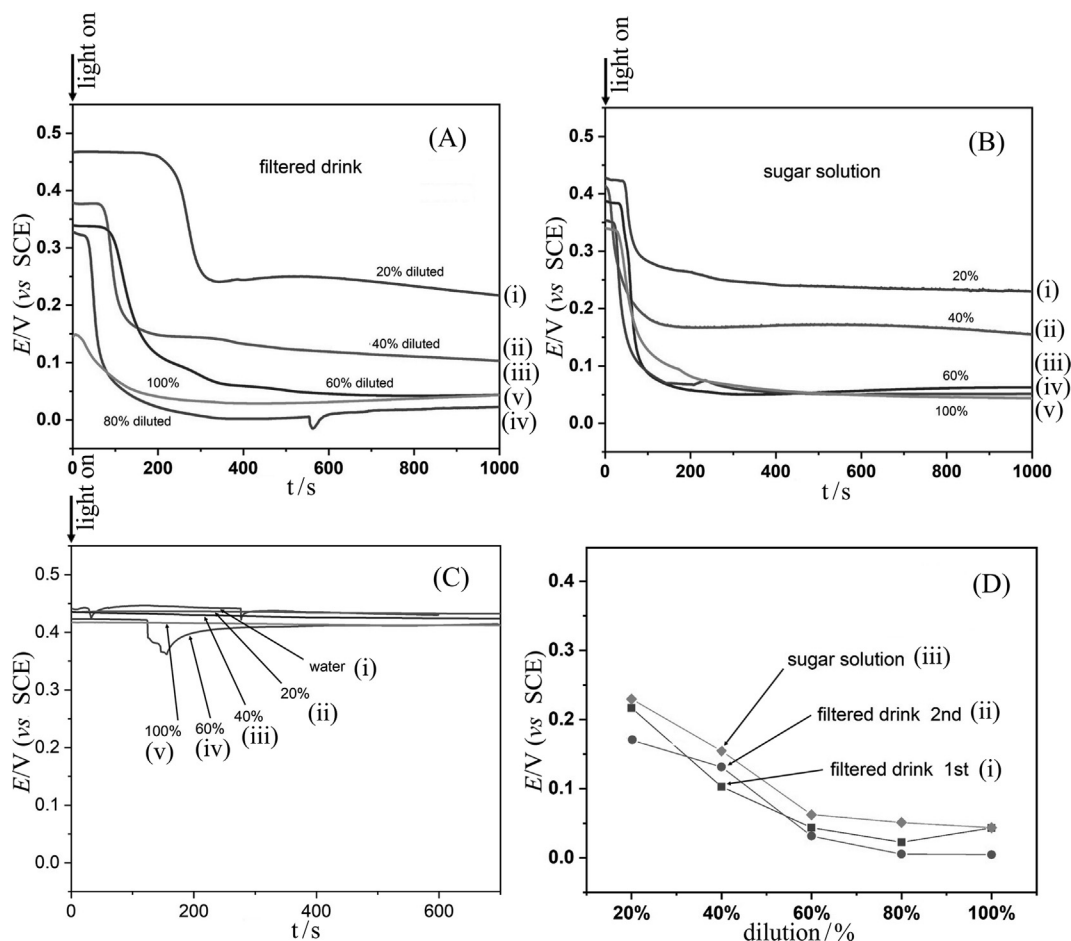


Fig. 5. (A) Chronopotentiometry (zero current) data for 60 μg Pt@g-C₃N₄ and 12 μg PIM-1 at a palladium membrane obtained for a filtered commercial soft drink containing a mixture of carbohydrates as a function of dilution. (B) As before, but for an aqueous solution of glucose:fructose:sucrose with molar ratio 1:4.95:2.42 and with total content of 0.35 g glucose + 1.75 g fructose + 1.30 g sucrose in 100 mL water to mimic the soft drink. (C) As before but for a filtered soft drink with artificial sweetener. (D) Plot of final equilibrium potential data (at 1000 s) for (i) the filtered drink, (ii) a repeat measurement for the filtered drink, and (iii) the artificial sugar solution as a function of dilution.

by approximately -50 mV. However, when argon de-aerating both sides of the palladium membrane, the final equilibrium potential with the softdrink approaches -0.2 V vs. SCE. Therefore, the conditions (oxygen content) on both sides of the palladium membrane during the analytical detection are important. Applications of this methodology seem most plausible for approximation/monitoring of total carbohydrate content in the presence of ambient oxygen. In future, improvements in the analytical performance are likely for example with thinner palladium composite membranes, with photo-chronoamperometric techniques, or based on voltammetric read-out of photocurrents.

4. Conclusions and outlook

It has been shown that a palladium film can be employed to separate an analyte compartment with glucose and an electrochemical compartment filled with aqueous 10 mM HCl. Production of hydrogen in the analyte compartment driven by a blue LED (385 nm) and catalysed by a Pt@g-C₃N₄ photocatalyst deposit causes the equilibrium potential of the palladium working electrode to respond. In future work, a wider range of photocatalysts and hydrogen evolution catalysts could be employed and tested, for example including materials based on oxygen deficient oxides [27].

A PIM-1 matrix for the Pt@g-C₃N₄ photocatalyst was employed to help capturing the hydrogen, protect against oxygen, and to provide a mechanically stable catalyst film. In the future, additional

work will be required to explore other types of PIM materials and more generally the robustness of this type of sensor. There are three potential failure modes based on (i) the photocatalyst failing, (ii) the palladium membrane becoming brittle, or (iii) the PIM-1 material itself undergoing degradation. Currently, there is no experimental data to predict the long levity of this type of indirect sensor in continuous operation.

When glucose was introduced as a hole quencher, significant photo-responses are recorded as change in equilibrium potential. The process is effective in distilled water, in commercial softdrink, or fruit juice samples. The measurable glucose concentrations range appeared to be from about 10 mM to approximately 300 mM in the presence of ambient oxygen. However, other types of carbohydrates such as fructose (reducing), or sucrose, trehalose (non-reducing) give photoresponses with similar characteristics. For commercial samples only the total content for a given mixtures of carbohydrates is measured. Distinguishing between the different types of quenchers is not possible under these conditions. Traditional techniques such as flow-through NMR or optical viscosity probes [28] could be employed as alternatively approaches. A biosensor array [29] for disaccharides and a flow injection biosensor based on enzymes to selectively/simultaneously detect glucose, fructose, and sucrose have been reported previously to monitor complex saccharide mixtures [30].

The "indirect electrochemical sensor" methodology is novel in that the separation of electrochemical and analysis compartments

allows the electrochemical detection to be separated from complex matrix elements (colloids, salts, additives, etc.). There is no requirement for the analyte to be conducting with electrolyte or buffered. Samples (biological or non-biological) can be monitored simply in contact to the membrane and exposed to blue light from an LED light source. In the future, a wider range of applications may be possible. However, the sensitivity as well as the response time of the sensor need to be improved for example by introducing much thinner types of membranes, or introducing alternative membranes based on graphene composites. Further applications beyond sensor development are possible in energy conversion and in waste-to-energy applications.

Declaration of Competing Interest

The authors declare that they have no known competing financial interests or personal relationships that could have appeared to influence the work reported in this paper.

Acknowledgements

Y.Z. thanks the China Scholarship Council (CSC scholarship No 20180935006) for a PhD scholarship. E.M., L.T.M., K.B., and F.M. thank EPSRC for support (EP/N013778/1).

References

- [1] L. Shi, Y. Yin, L.C. Zhang, S.B. Wang, M. Sillanpää, H.Q. Sun, Design and engineering heterojunctions for the photoelectrochemical monitoring of environmental pollutants: A review, *Appl. Catal. B-Environ.* 248 (2019) 405–422.
- [2] B. Sun, S.Y. Ai, Fabrication and application of photoelectrochemical sensor, *Progress Chem.* 26 (2014) 834–845.
- [3] L.T. Wey, P. Bombelli, X.L. Chen, J.M. Lawrence, C.M. Rabideau, S.J.L. Rowden, J. Z. Zhang, C.J. Howe, The development of biophotovoltaic systems for power generation and biological analysis, *ChemElectroChem* (2019), <https://doi.org/10.1002/celec.201900997>.
- [4] F.W.P. Ribeiro, F.C. Moraes, E.C. Pereira, F. Marken, L.H. Mascaro, New application for the BiVO₄ photoanode: A photoelectroanalytical sensor for nitrite, *Electrochem. Commun.* 61 (2015) 1–4.
- [5] S.Y. Yu, L. Zhang, L.B. Zhu, Y. Gao, G.C. Fan, D.M. Han, G.X. Chen, W.W. Zhao, Bismuth-containing semiconductors for photoelectrochemical sensing and biosensing, *Coordination Chem. Rev.* 393 (2019) 9–20.
- [6] B. Cakiroglu, M. Ozacar, A self-powered photoelectrochemical glucose biosensor based on supercapacitor Co₃O₄-CNT hybrid on TiO₂, *Biosens. Bioelectronics* 119 (2018) 34–41.
- [7] N.N. Fu, Y. Hu, S.H. Shi, S.K. Ren, W. Liu, S. Su, B.M. Zhao, L.X. Weng, L.H. Wang, Au nanoparticles on two-dimensional MoS₂ nanosheets as a photoanode for efficient photoelectrochemical miRNA detection, *Analyst* 143 (2018) 1705–1712.
- [8] N.N. Xu, T. Hou, F. Li, A label-free photoelectrochemical aptasensor for facile and ultrasensitive mercury ion assay based on a solution-phase photoactive probe and exonuclease III-assisted amplification, *Analyst* 144 (2019) 3800–3806.
- [9] J.A. Cooper, K.E. Woodhouse, A.M. Chippindale, R.G. Compton, Photoelectrochemical determination of ascorbic acid using methylene blue immobilized in alpha-zirconium phosphate, *Electroanalysis* 11 (1999) 1259–1265.
- [10] G.P. Dong, Y.H. Zhang, Q.W. Pan, J.R. Qiu, A fantastic graphitic carbon nitride (g-C₃N₄) material: Electronic structure, photocatalytic and photoelectronic properties, *J. Photochem. Photobiol. C-Photochem. Rev.* 20 (2014) 33–50.
- [11] F. Fina, H. Menard, J.T.S. Irvine, The effect of Pt NPs crystallinity and distribution on the photocatalytic activity of Pt-g-C₃N₄, *Phys. Chem. Chem. Phys.* 17 (2015) 13929–13936.
- [12] Y. Zheng, L.H. Lin, B. Wang, X.C. Wang, Graphitic carbon nitride polymers toward sustainable photoredox catalysis, *Angew. Chem. Inter. Ed.* 54 (2015) 12868–12884.
- [13] J.Q. Wen, J. Xie, X.B. Chen, X. Li, A review on g-C₃N₄-based photocatalysts, *Appl. Surf. Sci.* 391 (2017) 72–123.
- [14] Y.Z. Zhao, N.A. Al Abass, R. Malpass-Evans, M. Carta, N.B. McKeown, E. Madrid, P.J. Fletcher, F. Marken, Photoelectrochemistry of immobilised Pt@g-C₃N₄ mediated by hydrogen and enhanced by a polymer of intrinsic microporosity PIM-1, *Electrochem. Commun.* 103 (2019) 1–6.
- [15] F. Marken, E. Madrid, Y.Z. Zhao, M. Carta, N.B. McKeown, Polymers of intrinsic microporosity in triphasic electrochemistry: perspectives, *ChemElectroChem* 6 (2019) 4332–4342.
- [16] N.B. McKeown, P.M. Budd, Exploitation of intrinsic microporosity in polymer-based materials, *Macromolecules* 43 (2010) 5163–5176.
- [17] E. Madrid, N.B. McKeown, Innovative methods in electrochemistry based on polymers of intrinsic microporosity, *Curr. Opin. Electrochem.* 10 (2018) 61–66.
- [18] D.P. He, D.S. He, J.L. Yang, Z.X. Low, R. Malpass-Evans, M. Carta, N.B. McKeown, F. Marken, Molecularly rigid microporous polyamine captures and stabilizes conducting platinum nanoparticle networks, *ACS Appl. Mater. Interfaces* 8 (2016) 22425–22430.
- [19] E. Madrid, J.P. Lowe, K.J. Msayib, N.B. McKeown, Q.L. Song, G.A. Attard, T. Düren, F. Marken, Triphasic nature of polymers of intrinsic microporosity induces storage and catalysis effects in hydrogen and oxygen reactivity at electrode surfaces, *ChemElectroChem* 6 (2019) 252–259.
- [20] H.R. Kricheldorf, D. Fritsch, L. Vakhtangishvili, N. Lomadze, G. Schwarz, Cyclic ladder polymers based on 5,5'-, 6,6'-tetrahydroxy-3,3,3', 3'-tetramethylspirobisindane and 2,3,5,6-tetrafluoropyridines, *Macromolecules* 39 (2006) 4990–4998.
- [21] G.S. Larsen, P. Lin, K.E. Hart, C.M. Colina, Molecular simulations of PIM-1-like polymers of intrinsic microporosity, *Macromolecules* 44 (2011) 6944–6951.
- [22] P.M. Budd, E.S. Elabas, B.S. Ghanem, S. Makhseed, N.B. McKeown, K.J. Msayib, C. E. Tattershall, D. Wang, Solution-processed, organophilic membrane derived from a polymer of intrinsic microporosity, *Adv. Mater.* 16 (2004) 456–459.
- [23] R.S. Sherbo, R.S. Delima, V.A. Chiykowski, B.P. MacLeod, C.P. Berlinguette, Complete electron economy by pairing electrolysis with hydrogenation, *Nat. Catal.* 1 (2018) 501–507.
- [24] R.V. Bucur, Measurements of diffusion-coefficients of hydrogen in palladium by a galvanostatic permeation method, *Inter. J. Hydrogen Energy* 10 (1985) 399–405.
- [25] R.V. Bucur, The influence of experimental conditions upon the measurements of hydrogen diffusion in palladium by electrochemical permeation methods, *Zeitschrift Physikalische Chemie Neue Folge* 146 (1985) 217–229.
- [26] A. Naseri, M. Samadi, A. Pourjavadi, A.Z. Moshfegh, S. Ramakrishna, Graphitic carbon nitride (g-C₃N₄)-based photocatalysts for solar hydrogen generation: recent advances and future development directions, *J. Mater. Chem. A* 5 (2017) 23406–23433.
- [27] S. Liu, J. Zhu, M. Sun, Z. Ma, K. Hu, T. Nakajima, X. Liu, P. Schmuki, L. Wang, Promoting the hydrogen evolution reaction through oxygen vacancies and phase transformation engineering on layered double hydroxide nanosheets, *J. Mater. Chem. A* 8 (2020) 2490–2497.
- [28] A.D. Gomes, J. Kobelke, J. Bierlich, K. Schuster, H. Bartelt, O. Frazao, Optical fiber probe viscometer based on hollow capillary tube, *J. Lightwave Technol.* 37 (2019) 4456–4461.
- [29] T.E. Currey, M.A. Salazar, P. Oliveira, J. Javier, P.J. Dennis, P. Rao, J.B. Shear, Enzyme-based sensor arrays for rapid characterization of complex disaccharide solutions, *Anal. Biochem.* 303 (2002) 42–48.
- [30] J.K. Park, M.C. Shin, S.G. Lee, H.S. Kim, Flow-injection analysis of glucose, fructose, and sucrose using a biosensor constructed with permeabilized *zymomonas-mobilis* and invertase, *Biotechnol. Progress* 11 (1995) 58–63.